



# ALS Paragon



## GC/MS Volatiles Case Narrative

---

### **Colorado Oil & Gas Conservation Commission**

**Complaint 200204502**

**Work Order Number: 0903157**

1. This report consists of 1 water sample. The sample was received cool and intact by ALS Paragon on 03/20/09. All aqueous samples were free of headspace prior to analysis.
2. The sample was prepared according to SW-846, 3rd Edition procedures. Specifically, the water sample was prepared by purging 10 mL using purge and trap procedures based on Method 5030C.
3. The samples were analyzed using GC/MS with an RTX-624, RTX-VMS, or equivalent capillary column according to SOP 525 Revision 12 based on SW-846 Method 8260B. All positive results were quantitated against the initial calibration standards using the internal standard technique. The identification of positive results was achieved by a comparison of the retention time and mass spectrum of the sample versus the daily calibration standard.
4. All initial calibration criteria for SPCC's and CCC's were met. If average response factors were used in the initial calibration, %RSD was  $\leq 15\%$ . If linear or higher order regression calibrations were used in the initial calibration, the coefficient of determination ( $r^2$ )  $\geq 0.99$ .
5. All initial calibrations are verified by comparing a second source standard calibration verification (ICV) against the calibration curve. All target compounds in the second source verification had a %D of less than 25%.
6. All criteria for SPCC's and CCC's were met in daily (continuing) calibration verifications (CCV).
7. Methylene chloride, acetone and 2-butanone are common laboratory contaminants. In order to minimize the levels of these compounds detected in the gc/ms analysis, ALS Paragon has designated its volatile laboratory as a restricted access area. In addition, the laboratory has been equipped with a dedicated, air intake and exhaust system that operates under positive pressure in order to minimize cross contamination of these compounds. Due to fluctuations in ambient laboratory conditions, reported sample values for common laboratory contaminants may be due to lab contamination even if the compound in question is not detected in the associated method blank.

All method blank criteria were met.



8. All laboratory control sample and laboratory control sample duplicate recoveries and RPDs were within the acceptance criteria.
9. Since a sample from this order number was not the selected quality control (QC) sample, matrix specific QC results are not included in this report.
10. The sample was analyzed within the established holding time.
11. All surrogate recoveries were within acceptance criteria.
12. All internal standard recoveries were within acceptance criteria.
13. Manual integrations are performed when needed to provide consistent and defensible data following the guidelines in SOP 939 Revision 3.

The data contained in the following report have been reviewed and approved by the personnel listed below. In addition, ALS Paragon certifies that the analyses reported herein are true, complete and correct within the limits of the methods employed.

SY  
Sharon L. Jones  
Organics Primary Data Reviewer

3-29-09  
Date

Steven D. White  
Organics Final Data Reviewer

3-27-09  
Date



*ALS Paragon*  
*Data Qualifier Flags*  
*Chromatography and Mass Spectrometry*

<b>U or ND:</b>	<b>This flag indicates that the compound was analyzed for but not detected.</b>
<b>J:</b>	<b>This flag indicates an estimated value. This flag is used as follows : (1) when estimating a concentration for tentatively identified compounds (TICs) where a 1:1 response is assumed; (2) when the mass spectral and retention time data indicate the presence of a compound that meets the volatile and semivolatile GC/MS identification criteria, and the result is less than the reporting limit (RL) but greater than the method detection limit (MDL); (3) when the retention time data indicate the presence of a compound that meets the GC identification criteria, and the result is less than the RL but greater than the MDL; and (4) the reported value is estimated.</b>
<b>B:</b>	<b>This flag is used when the analyte is detected in the associated method blank as well as in the sample. It indicates probable blank contamination and warns the data user. This flag shall be used for a tentatively identified compound (TIC) as well as for a positively identified target compound.</b>
<b>E:</b>	<b>This flag identifies compounds whose concentration exceeds the upper level of the calibration range.</b>
<b>A:</b>	<b>This flag indicates that a tentatively identified compound is a suspected aldol-condensation product.</b>
<b>X:</b>	<b>This flag indicates that the analyte was diluted below an accurate quantitation level.</b>
<b>*:</b>	<b>This flag indicates that a spike recovery is equal to or outside the control criteria used.</b>
<b>+:</b>	<b>This flag indicates that the relative percent difference (RPD) equals or exceeds the control criteria.</b>

# ALS Paragon

## Sample Number(s) Cross-Reference Table

---

**Paragon OrderNum:** 0903157

**Client Name:** Colorado Oil & Gas Conservation Commission

**Client Project Name:** Complaint 200204502

**Client Project Number:**

**Client PO Number:** OE PHA 090000000004

---

Client Sample Number	Lab Sample Number	COC Number	Matrix	Date Collected	Time Collected
Pulsifer 090319	0903157-1		WATER	19-Mar-09	11:05

Project Name/No.: **AFR**

Sampler(s): **C. Whitmore**

Turnaround (circle one): **Standard**

or Rush (Due **14**)

Dispose: **30d**

Date

or Return to Client

Report To: **Peter Gintautas**

Phone: **719-846-3091**

Fax:

E-mail: **peter.gintautas@state.co.us**

Company: **Colo. Oil & Gas Services, Inc.**

Address:

Comments: **200204502**

**200204503**

Circle method (right); provide additional information as needed (comments).

Sample ID

Date

Time \*

Lab ID

Matrix

Preservative

(Indicate type... HCl, etc.)

No. of Containers

Sample ID	Date	Time *	Lab ID	Matrix	Preservative	(Indicate type... HCl, etc.)	No. of Containers
GORDON-090319	3/19/09	10:05	W				10
PULSIFER 090319		11:05					
VANAGESTIN 090319		12:40					
KOSSELIN 090319		13:45					

OC Pesticides

SW8081A

PCBs

SW8082

Herbicides

SW8151A

Explosives

SW8330

TCLP Organics

SW8260B 8270C 8081A 8151A

TCLP Metals

SW6010B 7470

Total Metals by ICP Hg

SW6010B 7470 7471 E200.7

Dissolved Metals by ICP Hg

SW6010B 7470 E200.7

Total Metals by ICP/MS

SW6020A E200.8

Dissolved Metals by ICP/MS \*

SW6020A E200.8

Hexavalent Chromium

SW706A E200.8

Inorganic Anions

SW9056 E300.0

Solids:

Total E160.3 TDS E160.1 TSS E160.2

pH

SW9040B SW9045C

Gross Alpha / Beta

SW9310 E900.0

Actinides by Paragon SOP

Pu / U / Am / Th / Cm /

Tritium

SW906.0

Total Alpha-Emitting Radium

SW9315 E903.0

Radium 226

E903.1

Radium 228

SW9320 E904.0

Strontium 90 (Total RadioSr)

D5811-00

Gamma Isotopes

E901.1

Radon 222

SM7510Rn

VOCs

SW8260B - 25 Full + TICS

BTEX (only)

SW8260B - 25 Full + TICS

SVOCs

SW8270C - Full + TICS

Relinquished By:

Signature

Printed Name

Date

Time

Relinquished By:

Signature

Printed Name

Date

Time

\* Time Zone: EST CST MST PST

Matrix Key: O = oil, S = soil, NS = non-soil solid, W = water, L = liquid, E = extract, F = filter

Comments:

Filter + preserve metals via receipt

ANIMS = Pb, Cl, F, NO<sub>3</sub>, NO<sub>2</sub>, SO<sub>4</sub>

200.7 = Ba, Be, B, Ca, Cr, Cu, Fe, Li, Mn, Mg, Ni, K, Na, Sr, Zn

200.6 = Sb, As, Cd, Pb, Mo, Se, Ag, Te, U

Form 20216.xls (6/16/08)

## CONDITION OF SAMPLE UPON RECEIPT FORM

Paragon Analytics

Client: COGCCWorkorder No: 0903157Project Manager: AWInitials: LJO Date: 3/20/09

1. Does this project require any <b>special handling</b> in addition to standard Paragon procedures?	YES	<input checked="" type="radio"/> NO
2. Are custody <b>seals</b> on <b>shipping containers</b> intact?	NONE	<input checked="" type="radio"/> YES NO
3. Are Custody seals on <b>sample containers</b> intact?	<input checked="" type="radio"/> NONE	YES NO
4. Is there a <b>COC (Chain-of-Custody)</b> present or other representative documents?	<input checked="" type="radio"/> YES	NO
5. Are the <b>COC and bottle labels complete and legible</b> ?	<input checked="" type="radio"/> YES	NO
6. Is the <b>COC in agreement</b> with samples received? (IDs, dates, times, no. of samples, no. of containers, matrix, requested analyses, etc.)	<input checked="" type="radio"/> YES	NO
7. Were <b>airbills / shipping documents</b> present and/or removable?	DROP OFF <input checked="" type="radio"/> YES	NO
8. Are all aqueous <b>samples requiring preservation preserved correctly?</b> (excluding volatiles)	N/A	<input checked="" type="radio"/> YES <input checked="" type="radio"/> NO
9. Are all aqueous <b>non-preserved samples pH 4-9</b> ?	N/A	<input checked="" type="radio"/> YES NO
10. Is there <b>sufficient sample</b> for the requested analyses?	<input checked="" type="radio"/> YES	NO
11. Were all samples placed in the <b>proper containers</b> for the requested analyses?	<input checked="" type="radio"/> YES	NO
12. Are all samples within <b>holding times</b> for the requested analyses?	<input checked="" type="radio"/> YES	NO
13. Were all sample containers received <b>intact?</b> (not broken or leaking, etc.)	<input checked="" type="radio"/> YES	NO
14. Are all samples requiring <b>no headspace (VOC, GRO, RSK/MEE, Rx CN/S, radon)</b> headspace free? <b>Size of bubble:</b> <u>    </u> < green pea <u>    </u> > green pea	N/A	<input checked="" type="radio"/> YES NO
15. Do perchlorate LCMS-MS samples <b>have</b> headspace? (at least 1/3 of container required)	<input checked="" type="radio"/> N/A	YES NO
16. Were samples checked for and free from the presence of <b>residual chlorine?</b> (Applicable when PM has indicated samples are from a chlorinated water source; note if field preservation with sodium thiosulfate was not observed.)	<input checked="" type="radio"/> N/A	YES NO
17. Were the samples <b>shipped on ice?</b>	<input checked="" type="radio"/> YES	NO
18. Were cooler temperatures measured at 0.1-6.0°C? <b>IR gun used*:</b> <input checked="" type="radio"/> #2 <input checked="" type="radio"/> #4 <b>RAD ONLY</b>	<input checked="" type="radio"/> YES	NO
Cooler #: <u>1</u>		
Temperature (°C): <u>2.2</u>		
No. of custody seals on cooler: <u>1</u>		
External µR/hr reading: <u>13</u>		
Background µR/hr reading: <u>11</u>		
Were external µR/hr readings ≤ two times background and within DOT acceptance criteria? <input checked="" type="radio"/> YES <input checked="" type="radio"/> NO / NA (If no. see Form 008.)		

Additional Information: PROVIDE DETAILS BELOW FOR A NO RESPONSE TO ANY QUESTION ABOVE, EXCEPT #1 AND #16.

\* Sample 1, the 1L amber for SVOC analysis listed no sample time.  
 • The 500ml poly for metals analysis needs to be filtered and preserved in house.

If applicable, was the client contacted? YES / NO / NA Contact:                      Date/Time:                     Project Manager Signature / Date:                      3/23/09

\*IR Gun #2: Oakton, SN 29922500201-0066

\*IR Gun #4: Oakton, SN 2372220101-0002

# GC/MS Volatiles

Method SW8260\_25B

Method Blank

Lab Name: ALS Paragon

Work Order Number: 0903157

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204502

Lab ID: VL090323-3MB

Sample Matrix: WATER

% Moisture: N/A

Date Collected: N/A

Date Extracted: 23-Mar-09

Date Analyzed: 23-Mar-09

Prep Method: SW5030 Rev C

Prep Batch: VL090323-3

QCBatchID: VL090323-3-1

Run ID: VL090323-3A

Cleanup: NONE

Basis: N/A

File Name: C13948

Sample Aliquot: 10 ml

Final Volume: 10 ml

Result Units: UG/L

Clean DF: 1

CASNO	Target Analyte	DF	Result	Reporting Limit	Result Qualifier	EPA Qualifier
75-71-8	DICHLORODIFLUOROMETHANE	1	1	1	U	
74-87-3	CHLOROMETHANE	1	1	1	U	
75-01-4	VINYL CHLORIDE	1	1	1	U	
74-83-9	BROMOMETHANE	1	1	1	U	
75-00-3	CHLOROETHANE	1	1	1	U	
75-69-4	TRICHLOROFLUOROMETHANE	1	1	1	U	
75-35-4	1,1-DICHLOROETHENE	1	1	1	U	
76-13-1	1,1,2-TRICHLORO-1,2,2-TRIFLUOROET	1	1	1	U	
67-64-1	ACETONE	1	10	10	U	
74-88-4	IODOMETHANE	1	1	1	U	
75-15-0	CARBON DISULFIDE	1	1	1	U	
75-09-2	METHYLENE CHLORIDE	1	1	1	U	
156-60-5	TRANS-1,2-DICHLOROETHENE	1	1	1	U	
1634-04-4	METHYL TERTIARY BUTYL ETHER	1	1	1	U	
75-34-3	1,1-DICHLOROETHANE	1	1	1	U	
108-05-4	VINYL ACETATE	1	2	2	U	
156-59-2	CIS-1,2-DICHLOROETHENE	1	1	1	U	
78-93-3	2-BUTANONE	1	10	10	U	
74-97-5	BROMOCHLOROMETHANE	1	1	1	U	
67-66-3	CHLOROFORM	1	1	1	U	
71-55-6	1,1,1-TRICHLOROETHANE	1	1	1	U	
594-20-7	2,2-DICHLOROPROPANE	1	1	1	U	
56-23-5	CARBON TETRACHLORIDE	1	1	1	U	
563-58-6	1,1-DICHLOROPROPENE	1	1	1	U	
107-06-2	1,2-DICHLOROETHANE	1	1	1	U	
71-43-2	BENZENE	1	1	1	U	
79-01-6	TRICHLOROETHENE	1	1	1	U	

Data Package ID: VL0903157-1

Date Printed: Thursday, March 26, 2009

ALS Paragon

LIMS Version: 6.252A

Page 1 of 3

# GC/MS Volatiles

Method SW8260\_25B

Method Blank

Lab Name: ALS Paragon

Work Order Number: 0903157

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204502

Lab ID: VL090323-3MB

Sample Matrix: WATER

% Moisture: N/A

Date Collected: N/A

Date Extracted: 23-Mar-09

Date Analyzed: 23-Mar-09

Prep Method: SW5030 Rev C

Prep Batch: VL090323-3

QCBatchID: VL090323-3-1

Run ID: VL090323-3A

Cleanup: NONE

Basis: N/A

File Name: C13948

Sample Aliquot: 10 ml

Final Volume: 10 ml

Result Units: UG/L

Clean DF: 1

78-87-5	1,2-DICHLOROPROPANE	1	1	1	U	
74-95-3	DIBROMOMETHANE	1	1	1	U	
75-27-4	BROMODICHLOROMETHANE	1	1	1	U	
10061-01-5	CIS-1,3-DICHLOROPROPENE	1	1	1	U	
108-10-1	4-METHYL-2-PENTANONE	1	10	10	U	
108-88-3	TOLUENE	1	1	1	U	
10061-02-6	TRANS-1,3-DICHLOROPROPENE	1	1	1	U	
79-00-5	1,1,2-TRICHLOROETHANE	1	1	1	U	
591-78-6	2-HEXANONE	1	10	10	U	
127-18-4	TETRACHLOROETHENE	1	1	1	U	
142-28-9	1,3-DICHLOROPROPANE	1	1	1	U	
124-48-1	DIBROMOCHLOROMETHANE	1	1	1	U	
106-93-4	1,2-DIBROMOETHANE	1	1	1	U	
544-10-5	1-CHLOROHEXANE	1	1	1	U	
108-90-7	CHLOROBENZENE	1	1	1	U	
630-20-6	1,1,1,2-TETRACHLOROETHANE	1	1	1	U	
100-41-4	ETHYLBENZENE	1	1	1	U	
136777-61-2	M+P-XYLENE	1	1	1	U	
95-47-6	O-XYLENE	1	1	1	U	
100-42-5	STYRENE	1	1	1	U	
75-25-2	BROMOFORM	1	1	1	U	
98-82-8	ISOPROPYLBENZENE	1	1	1	U	
96-18-4	1,2,3-TRICHLOROPROPANE	1	1	1	U	
79-34-5	1,1,2,2-TETRACHLOROETHANE	1	1	1	U	
108-86-1	BROMOBENZENE	1	1	1	U	
103-65-1	N-PROPYLBENZENE	1	1	1	U	
95-49-8	2-CHLOROTOLUENE	1	1	1	U	
108-67-8	1,3,5-TRIMETHYLBENZENE	1	1	1	U	
106-43-4	4-CHLOROTOLUENE	1	1	1	U	

Data Package ID: VL0903157-1

Date Printed: Thursday, March 26, 2009

ALS Paragon

LIMS Version: 6.252A

Page 2 of 3



# GC/MS Volatiles

Method SW8260\_25B

Method Blank

Lab Name: ALS Paragon

Work Order Number: 0903157

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204502

Lab ID: VL090323-3MB

Sample Matrix: WATER

% Moisture: N/A

Date Collected: N/A

Date Extracted: 23-Mar-09

Date Analyzed: 23-Mar-09

Prep Method: SW5030 Rev C

Prep Batch: VL090323-3

QCBatchID: VL090323-3-1

Run ID: VL090323-3A

Cleanup: NONE

Basis: N/A

File Name: C13948

Sample Aliquot: 10 ml

Final Volume: 10 ml

Result Units: UG/L

Clean DF: 1

98-06-6	TERT-BUTYLBENZENE	1	1	1	U	
95-63-6	1,2,4-TRIMETHYLBENZENE	1	1	1	U	
135-98-8	SEC-BUTYLBENZENE	1	1	1	U	
541-73-1	1,3-DICHLOROBENZENE	1	1	1	U	
99-87-6	P-ISOPROPYLTOLUENE	1	1	1	U	
106-46-7	1,4-DICHLOROBENZENE	1	1	1	U	
104-51-8	N-BUTYLBENZENE	1	1	1	U	
95-50-1	1,2-DICHLOROBENZENE	1	1	1	U	
96-12-8	1,2-DIBROMO-3-CHLOROPROPANE	1	2	2	U	
120-82-1	1,2,4-TRICHLOROBENZENE	1	1	1	U	
87-68-3	HEXACHLOROBUTADIENE	1	1	1	U	
91-20-3	NAPHTHALENE	1	1	1	U	
87-61-6	1,2,3-TRICHLOROBENZENE	1	1	1	U	

## Surrogate Recovery

CASNO	Surrogate Analyte	Result	Flag	Spike Amount	Percent Recovery	Control Limits
460-00-4	4-BROMOFLUOROBENZENE	26.3		25	105	78 - 129
1868-53-7	DIBROMOFLUOROMETHANE	24.9		25	100	80 - 124
2037-26-5	TOLUENE-D8	26		25	104	81 - 119

Data Package ID: VL0903157-1

Date Printed: Thursday, March 26, 2009

ALS Paragon

LIMS Version: 6.252A

Page 3 of 3

# GC/MS Volatiles

Method SW8260\_25

## Tentatively Identified Compounds

Lab Name: ALS Paragon

Work Order Number: 0903157

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204502

Field ID:	
Lab ID:	VL090323-3MB

Sample Matrix: WATER

% Moisture: N/A

Date Collected: N/A

Date Extracted: 23-Mar-09

Date Analyzed: 23-Mar-09

Prep Batch: VL090323-3

QCBatchID: VL090323-3-1

Run ID: VL090323-3A

Cleanup: NONE

Basis: As Received

Sample Aliquot: 10 ml

Final Volume: 10 ml

Clean DF: 1

File Name: C13948

CASNO	Retention Time	Target Analyte	Dilution Factor	Result	Units	Qualifier
128-37-0	14.17	BUTYLATED HYDROXYTOLUENE	1	3.9	UG/L	J

Data Package ID: VL0903157-1

Date Printed: Thursday, March 26, 2009

ALS Paragon

LIMS Version: 6.252A

Page 2 of 2

# GC/MS Volatiles

Method SW8260\_25B

## Sample Results

Lab Name: ALS Paragon

Work Order Number: 0903157

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204502

Field ID:	Pulsifer 090319	Sample Matrix:	WATER	Prep Batch:	VL090323-3	Sample Aliquot:	10 ml
Lab ID:	0903157-1	% Moisture:	N/A	QCBatchID:	VL090323-3-1	Final Volume:	10 ml
		Date Collected:	19-Mar-09	Run ID:	VL090323-3A	Result Units:	UG/L
		Date Extracted:	23-Mar-09	Cleanup:	NONE	Clean DF:	1
		Date Analyzed:	23-Mar-09	Basis:	As Received		
		Prep Method:	SW5030 Rev C	File Name:	C13955		

CASNO	Target Analyte	Dilution Factor	Result	Reporting Limit	Result Qualifier	EPA Qualifier
75-71-8	DICHLORODIFLUOROMETHANE	1	1	1	U	
74-87-3	CHLOROMETHANE	1	1	1	U	
75-01-4	VINYL CHLORIDE	1	1	1	U	
74-83-9	BROMOMETHANE	1	1	1	U	
75-00-3	CHLOROETHANE	1	1	1	U	
75-69-4	TRICHLOROFLUOROMETHANE	1	1	1	U	
75-35-4	1,1-DICHLOROETHENE	1	1	1	U	
76-13-1	1,1,2-TRICHLORO-1,2,2-TRIFLUOROETHANE	1	1	1	U	
67-64-1	ACETONE	1	10	10	U	
74-88-4	IODOMETHANE	1	1	1	U	
75-15-0	CARBON DISULFIDE	1	1	1	U	
75-09-2	METHYLENE CHLORIDE	1	1	1	U	
156-60-5	TRANS-1,2-DICHLOROETHENE	1	1	1	U	
1634-04-4	METHYL TERTIARY BUTYL ETHER	1	1	1	U	
75-34-3	1,1-DICHLOROETHANE	1	1	1	U	
108-05-4	VINYL ACETATE	1	2	2	U	
156-59-2	CIS-1,2-DICHLOROETHENE	1	1	1	U	
78-93-3	2-BUTANONE	1	10	10	U	
74-97-5	BROMOCHLOROMETHANE	1	1	1	U	
67-66-3	CHLOROFORM	1	1	1	U	
71-55-6	1,1,1-TRICHLOROETHANE	1	1	1	U	
594-20-7	2,2-DICHLOROPROPANE	1	1	1	U	
56-23-5	CARBON TETRACHLORIDE	1	1	1	U	
563-58-6	1,1-DICHLOROPROPENE	1	1	1	U	
107-06-2	1,2-DICHLOROETHANE	1	1	1	U	
71-43-2	BENZENE	1	1	1	U	
79-01-6	TRICHLOROETHENE	1	1	1	U	

Data Package ID: VL0903157-1

Date Printed: Thursday, March 26, 2009

ALS Paragon

Page 1 of 3

LIMS Version: 6.252A

# GC/MS Volatiles

Method SW8260\_25B

## Sample Results

Lab Name: ALS Paragon

Work Order Number: 0903157

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204502

Field ID:	Pulsifer 090319
Lab ID:	0903157-1

Sample Matrix: WATER

% Moisture: N/A

Date Collected: 19-Mar-09

Date Extracted: 23-Mar-09

Date Analyzed: 23-Mar-09

Prep Method: SW5030 Rev C

Prep Batch: VL090323-3

QCBatchID: VL090323-3-1

Run ID: VL090323-3A

Cleanup: NONE

Basis: As Received

File Name: C13955

Sample Aliquot: 10 ml

Final Volume: 10 ml

Result Units: UG/L

Clean DF: 1

78-87-5	1,2-DICHLOROPROPANE	1	1	1	U	
74-95-3	DIBROMOMETHANE	1	1	1	U	
75-27-4	BROMODICHLOROMETHANE	1	1	1	U	
10061-01-5	CIS-1,3-DICHLOROPROPENE	1	1	1	U	
108-10-1	4-METHYL-2-PENTANONE	1	10	10	U	
108-88-3	TOLUENE	1	1	1	U	
10061-02-6	TRANS-1,3-DICHLOROPROPENE	1	1	1	U	
79-00-5	1,1,2-TRICHLOROETHANE	1	1	1	U	
591-78-6	2-HEXANONE	1	10	10	U	
127-18-4	TETRACHLOROETHENE	1	1	1	U	
142-28-9	1,3-DICHLOROPROPANE	1	1	1	U	
124-48-1	DIBROMOCHLOROMETHANE	1	1	1	U	
106-93-4	1,2-DIBROMOETHANE	1	1	1	U	
544-10-5	1-CHLOROHEXANE	1	1	1	U	
108-90-7	CHLOROBENZENE	1	1	1	U	
630-20-6	1,1,1,2-TETRACHLOROETHANE	1	1	1	U	
100-41-4	ETHYLBENZENE	1	1	1	U	
136777-61-2	M+P-XYLENE	1	1	1	U	
95-47-6	O-XYLENE	1	1	1	U	
100-42-5	STYRENE	1	1	1	U	
75-25-2	BROMOFORM	1	1	1	U	
98-82-8	ISOPROPYLBENZENE	1	1	1	U	
96-18-4	1,2,3-TRICHLOROPROPANE	1	1	1	U	
79-34-5	1,1,2,2-TETRACHLOROETHANE	1	1	1	U	
108-86-1	BROMOBENZENE	1	1	1	U	
103-65-1	N-PROPYLBENZENE	1	1	1	U	
95-49-8	2-CHLOROTOLUENE	1	1	1	U	
108-67-8	1,3,5-TRIMETHYLBENZENE	1	1	1	U	
106-43-4	4-CHLOROTOLUENE	1	1	1	U	

Data Package ID: VL0903157-1

Date Printed: Thursday, March 26, 2009

ALS Paragon

LIMS Version: 6.252A

Page 2 of 3

# GC/MS Volatiles

Method SW8260\_25B

## Sample Results

Lab Name: ALS Paragon

Work Order Number: 0903157

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204502

Field ID:	Pulsifer 090319
Lab ID:	0903157-1

Sample Matrix: WATER  
% Moisture: N/A  
Date Collected: 19-Mar-09  
Date Extracted: 23-Mar-09  
Date Analyzed: 23-Mar-09  
Prep Method: SW5030 Rev C

Prep Batch: VL090323-3  
QCBatchID: VL090323-3-1  
Run ID: VL090323-3A  
Cleanup: NONE  
Basis: As Received  
File Name: C13955

Sample Aliquot: 10 ml  
Final Volume: 10 ml  
Result Units: UG/L  
Clean DF: 1

98-06-6	TERT-BUTYLBENZENE	1	1	1	U	
95-63-6	1,2,4-TRIMETHYLBENZENE	1	1	1	U	
135-98-8	SEC-BUTYLBENZENE	1	1	1	U	
541-73-1	1,3-DICHLOROBENZENE	1	1	1	U	
99-87-6	P-ISOPROPYLTOLUENE	1	1	1	U	
106-46-7	1,4-DICHLOROBENZENE	1	1	1	U	
104-51-8	N-BUTYLBENZENE	1	1	1	U	
95-50-1	1,2-DICHLOROBENZENE	1	1	1	U	
96-12-8	1,2-DIBROMO-3-CHLOROPROPANE	1	2	2	U	
120-82-1	1,2,4-TRICHLOROBENZENE	1	1	1	U	
87-68-3	HEXACHLOROBUTADIENE	1	1	1	U	
91-20-3	NAPHTHALENE	1	1	1	U	
87-61-6	1,2,3-TRICHLOROBENZENE	1	1	1	U	

## Surrogate Recovery

CASNO	Surrogate Analyte	Result	Flag	Spike Amount	Percent Recovery	Control Limits
460-00-4	4-BROMOFLUOROBENZENE	25.8		25	103	78 - 129
1868-53-7	DIBROMOFLUOROMETHANE	26.4		25	105	80 - 124
2037-26-5	TOLUENE-D8	25.4		25	102	81 - 119

Data Package ID: VL0903157-1

Date Printed: Thursday, March 26, 2009

ALS Paragon

LIMS Version: 6.252A

Page 3 of 3

# GC/MS Volatiles

Method SW8260\_25

## Tentatively Identified Compounds

Lab Name: ALS Paragon

Work Order Number: 0903157

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204502

Field ID:	Pulsifer 090319
Lab ID:	0903157-1

Sample Matrix: WATER

% Moisture: N/A

Date Collected: 19-Mar-09

Date Extracted: 23-Mar-09

Date Analyzed: 23-Mar-09

Prep Batch: VL090323-3

QCBatchID: VL090323-3-1

Run ID: VL090323-3A

Cleanup: NONE

Basis: As Received

Sample Aliquot: 10 ml

Final Volume: 10 ml

Clean DF: 1

File Name: C13955

CASNO	Retention Time	Target Analyte	Dilution Factor	Result	Units	Qualifier
	3.37	UNKNOWN1	1	2.6	UG/L	J
	3.66	UNKNOWN2	1	1.8	UG/L	J
110-82-7	8.58	Cyclohexane	1	1.1	UG/L	J

Data Package ID: VL0903157-1

Date Printed: Thursday, March 26, 2009

ALS Paragon

LIMS Version: 6.252A

Page 1 of 2

# GC/MS Volatiles

Method SW8260\_25B

## Laboratory Control Sample and Laboratory Control Sample Duplicate

Lab Name: ALS Paragon

Work Order Number: 0903157

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204502

Lab ID: VL090323-3LCS

Sample Matrix: WATER

% Moisture: N/A

Date Collected: N/A

Date Extracted: 03/23/2009

Date Analyzed: 03/23/2009

Prep Method: SW5030C

Prep Batch: VL090323-3

QCBatchID: VL090323-3-1

Run ID: VL090323-3A

Cleanup: NONE

Basis: N/A

File Name: C13945

Sample Aliquot: 10 ml

Final Volume: 10 ml

Result Units: UG/L

Clean DF: 1

CASNO	Target Analyte	Spike Added	LCS Result	Reporting Limit	Result Qualifier	LCS % Rec.	Control Limits
75-71-8	DICHLORODIFLUOROMETHANE	10	9.73	1		97	38 - 131%
74-87-3	CHLOROMETHANE	10	9.57	1		96	62 - 141%
75-01-4	VINYL CHLORIDE	10	9.79	1		98	77 - 124%
74-83-9	BROMOMETHANE	10	10.5	1		105	76 - 133%
75-00-3	CHLOROETHANE	10	9.7	1		97	81 - 130%
75-69-4	TRICHLOROFLUOROMETHANE	10	10	1		100	84 - 146%
75-35-4	1,1-DICHLOROETHENE	10	10.2	1		102	75 - 126%
76-13-1	1,1,2-TRICHLORO-1,2,2-TRIFLUOROETHA	10	10.3	1		103	71 - 144%
67-64-1	ACETONE	40	34.5	10		86	50 - 150%
74-88-4	IODOMETHANE	10	10.5	1		105	76 - 116%
75-15-0	CARBON DISULFIDE	10	10.2	1		102	68 - 129%
75-09-2	METHYLENE CHLORIDE	10	9.46	1		95	22 - 146%
156-60-5	TRANS-1,2-DICHLOROETHENE	10	10.5	1		105	76 - 135%
1634-04-4	METHYL TERTIARY BUTYL ETHER	20	16.9	1		85	75 - 125%
75-34-3	1,1-DICHLOROETHANE	10	10.2	1		102	77 - 131%
108-05-4	VINYL ACETATE	10	9.82	2		98	56 - 151%
156-59-2	CIS-1,2-DICHLOROETHENE	10	10.3	1		103	81 - 121%
78-93-3	2-BUTANONE	40	34.2	10		85	50 - 150%
74-97-5	BROMOCHLOROMETHANE	10	9.65	1		96	85 - 126%
67-66-3	CHLOROFORM	10	10.3	1		103	84 - 125%
71-55-6	1,1,1-TRICHLOROETHANE	10	10.4	1		104	82 - 129%
594-20-7	2,2-DICHLOROPROPANE	10	11.7	1		117	79 - 130%
56-23-5	CARBON TETRACHLORIDE	10	10.7	1		107	83 - 135%
563-58-6	1,1-DICHLOROPROPENE	10	10.6	1		106	85 - 127%
107-06-2	1,2-DICHLOROETHANE	10	9.35	1		94	84 - 126%
71-43-2	BENZENE	10	10	1		100	82 - 122%

Data Package ID: VL0903157-1

Date Printed: Thursday, March 26, 2009

ALS Paragon

LIMS Version: 6.252A

Page 1 of 6

# GC/MS Volatiles

Method SW8260\_25B

## Laboratory Control Sample and Laboratory Control Sample Duplicate

Lab Name: ALS Paragon

Work Order Number: 0903157

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204502

Lab ID: VL090323-3LCS

Sample Matrix: WATER

% Moisture: N/A

Date Collected: N/A

Date Extracted: 03/23/2009

Date Analyzed: 03/23/2009

Prep Method: SW5030C

Prep Batch: VL090323-3

QCBatchID: VL090323-3-1

Run ID: VL090323-3A

Cleanup: NONE

Basis: N/A

File Name: C13945

Sample Aliquot: 10 ml

Final Volume: 10 ml

Result Units: UG/L

Clean DF: 1

CASNO	Target Analyte	Spike Added	LCS Result	Reporting Limit	Result Qualifier	LCS % Rec.	Control Limits
79-01-6	TRICHLOROETHENE	10	10.1	1		101	82 - 121%
78-87-5	1,2-DICHLOROPROPANE	10	9.81	1		98	81 - 121%
74-95-3	DIBROMOMETHANE	10	9.15	1		91	81 - 125%
75-27-4	BROMODICHLOROMETHANE	10	9.98	1		100	82 - 120%
10061-01-5	CIS-1,3-DICHLOROPROPENE	10	10.1	1		101	79 - 120%
108-10-1	4-METHYL-2-PENTANONE	40	32.7	10		82	50 - 150%
108-88-3	TOLUENE	10	10.9	1		109	83 - 121%
10061-02-6	TRANS-1,3-DICHLOROPROPENE	10	10.2	1		102	78 - 113%
79-00-5	1,1,2-TRICHLOROETHANE	10	9.74	1		97	82 - 122%
591-78-6	2-HEXANONE	40	34.7	10		87	50 - 150%
127-18-4	TETRACHLOROETHENE	10	11.3	1		113	79 - 136%
142-28-9	1,3-DICHLOROPROPANE	10	9.79	1		98	80 - 126%
124-48-1	DIBROMOCHLOROMETHANE	10	9.78	1		98	80 - 123%
106-93-4	1,2-DIBROMOETHANE	10	9.49	1		95	85 - 124%
544-10-5	1-CHLOROHEXANE	10	11.1	1		111	77 - 135%
108-90-7	CHLOROBENZENE	10	10.8	1		108	82 - 121%
630-20-6	1,1,1,2-TETRACHLOROETHANE	10	10.6	1		106	85 - 128%
100-41-4	ETHYLBENZENE	10	11.1	1		111	83 - 126%
136777-61-	M+P-XYLENE	20	22.2	1		111	82 - 129%
95-47-6	O-XYLENE	10	11.2	1		112	87 - 132%
100-42-5	STYRENE	10	10.9	1		109	82 - 123%
75-25-2	BROMOFORM	10	9.52	1		95	79 - 118%
98-82-8	ISOPROPYLBENZENE	10	11.2	1		112	75 - 132%
96-18-4	1,2,3-TRICHLOROPROPANE	10	9.46	1		95	77 - 128%
79-34-5	1,1,2,2-TETRACHLOROETHANE	10	9.73	1		97	74 - 130%
108-86-1	BROMOBENZENE	10	10.7	1		107	78 - 124%
103-65-1	N-PROPYLBENZENE	10	11.6	1		116	75 - 134%

Data Package ID: VL0903157-1

Date Printed: Thursday, March 26, 2009

ALS Paragon

LIMS Version: 6.252A

Page 2 of 6



# GC/MS Volatiles

Method SW8260\_25B

## Laboratory Control Sample and Laboratory Control Sample Duplicate

Lab Name: ALS Paragon

Work Order Number: 0903157

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204502

Lab ID: VL090323-3LCS

Sample Matrix: WATER

% Moisture: N/A

Date Collected: N/A

Date Extracted: 03/23/2009

Date Analyzed: 03/23/2009

Prep Method: SW5030C

Prep Batch: VL090323-3

QCBatchID: VL090323-3-1

Run ID: VL090323-3A

Cleanup: NONE

Basis: N/A

File Name: C13945

Sample Aliquot: 10 ml

Final Volume: 10 ml

Result Units: UG/L

Clean DF: 1

CASNO	Target Analyte	Spike Added	LCS Result	Reporting Limit	Result Qualifier	LCS % Rec.	Control Limits
95-49-8	2-CHLOROTOLUENE	10	11.5	1		115	77 - 128%
108-67-8	1,3,5-TRIMETHYLBENZENE	10	11.7	1		117	77 - 131%
106-43-4	4-CHLOROTOLUENE	10	11.3	1		113	79 - 128%
98-06-6	TERT-BUTYLBENZENE	10	11.8	1		118	76 - 134%
95-63-6	1,2,4-TRIMETHYLBENZENE	10	11.2	1		112	80 - 138%
135-98-8	SEC-BUTYLBENZENE	10	11.4	1		114	73 - 135%
541-73-1	1,3-DICHLOROBENZENE	10	11.1	1		111	79 - 126%
99-87-6	P-ISOPROPYLTOLUENE	10	11.5	1		115	72 - 132%
106-46-7	1,4-DICHLOROBENZENE	10	10.4	1		104	81 - 125%
104-51-8	N-BUTYLBENZENE	10	11.9	1		119	77 - 141%
95-50-1	1,2-DICHLOROBENZENE	10	10.5	1		105	82 - 128%
96-12-8	1,2-DIBROMO-3-CHLOROPROPANE	10	9.41	2		94	64 - 134%
120-82-1	1,2,4-TRICHLOROBENZENE	10	10.3	1		103	80 - 128%
87-68-3	HEXACHLOROBUTADIENE	10	11.7	1		117	70 - 136%
91-20-3	NAPHTHALENE	10	10.1	1		101	78 - 125%
87-61-6	1,2,3-TRICHLOROBENZENE	10	10.2	1		102	79 - 131%

Data Package ID: VL0903157-1

Date Printed: Thursday, March 26, 2009

ALS Paragon

LIMS Version: 6.252A

Page 3 of 6

# GC/MS Volatiles

Method SW8260\_25B

## Laboratory Control Sample and Laboratory Control Sample Duplicate

Lab Name: ALS Paragon

Work Order Number: 0903157

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204502

Lab ID: VL090323-3LCSD

Sample Matrix: WATER

% Moisture: N/A

Date Collected: N/A

Date Extracted: 03/23/2009

Date Analyzed: 03/23/2009

Prep Method: SW5030C

Prep Batch: VL090323-3

QCBatchID: VL090323-3-1

Run ID: VL090323-3A

Cleanup: NONE

Basis: N/A

File Name: C13946

Sample Aliquot: 10 ml

Final Volume: 10 ml

Result Units: UG/L

Clean DF: 1

CASNO	Target Analyte	Spike Added	LCSD Result	Reporting Limit	Result Qualifier	LCSD % Rec.	RPD Limit	RPD
75-71-8	DICHLORODIFLUOROMETHANE	10	9.86	1		99	20	1
74-87-3	CHLOROMETHANE	10	9.76	1		98	20	2
75-01-4	VINYL CHLORIDE	10	9.67	1		97	20	1
74-83-9	BROMOMETHANE	10	10.5	1		105	20	0
75-00-3	CHLOROETHANE	10	9.84	1		98	20	1
75-69-4	TRICHLOROFLUOROMETHANE	10	9.68	1		97	20	4
75-35-4	1,1-DICHLOROETHENE	10	10.1	1		101	20	1
76-13-1	1,1,2-TRICHLORO-1,2,2-TRIFLUOROETHA	10	10.4	1		104	20	1
67-64-1	ACETONE	40	38.1	10		95	30	10
74-88-4	IODOMETHANE	10	10.3	1		103	20	2
75-15-0	CARBON DISULFIDE	10	10	1		100	20	2
75-09-2	METHYLENE CHLORIDE	10	9.8	1		98	20	3
156-60-5	TRANS-1,2-DICHLOROETHENE	10	10.5	1		105	20	0
1634-04-4	METHYL TERTIARY BUTYL ETHER	20	18.9	1		94	20	11
75-34-3	1,1-DICHLOROETHANE	10	10.1	1		101	20	0
108-05-4	VINYL ACETATE	10	11	2		110	20	12
156-59-2	CIS-1,2-DICHLOROETHENE	10	10.3	1		103	20	0
78-93-3	2-BUTANONE	40	38.4	10		96	30	12
74-97-5	BROMOCHLOROMETHANE	10	10.3	1		103	20	7
67-66-3	CHLOROFORM	10	10.4	1		104	20	1
71-55-6	1,1,1-TRICHLOROETHANE	10	10.4	1		104	20	0
594-20-7	2,2-DICHLOROPROPANE	10	11.6	1		116	20	1
56-23-5	CARBON TETRACHLORIDE	10	10.5	1		105	20	2
563-58-6	1,1-DICHLOROPROPENE	10	10.4	1		104	20	2
107-06-2	1,2-DICHLOROETHANE	10	9.93	1		99	20	6
71-43-2	BENZENE	10	10.2	1		102	20	1
79-01-6	TRICHLOROETHENE	10	10.4	1		104	20	3

Data Package ID: VL0903157-1

Date Printed: Thursday, March 26, 2009

ALS Paragon

LIMS Version: 6.252A

Page 4 of 6

# GC/MS Volatiles

Method SW8260\_25B

## Laboratory Control Sample and Laboratory Control Sample Duplicate

Lab Name: ALS Paragon

Work Order Number: 0903157

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204502

Lab ID: VL090323-3LCSD

Sample Matrix: WATER

% Moisture: N/A

Date Collected: N/A

Date Extracted: 03/23/2009

Date Analyzed: 03/23/2009

Prep Method: SW5030C

Prep Batch: VL090323-3

QCBatchID: VL090323-3-1

Run ID: VL090323-3A

Cleanup: NONE

Basis: N/A

File Name: C13946

Sample Aliquot: 10 ml

Final Volume: 10 ml

Result Units: UG/L

Clean DF: 1

CASNO	Target Analyte	Spike Added	LCSD Result	Reporting Limit	Result Qualifier	LCSD % Rec.	RPD Limit	RPD
78-87-5	1,2-DICHLOROPROPANE	10	10.4	1		104	20	6
74-95-3	DIBROMOMETHANE	10	9.96	1		100	20	8
75-27-4	BROMODICHLOROMETHANE	10	10.6	1		106	20	6
10061-01-5	CIS-1,3-DICHLOROPROPENE	10	10.7	1		107	20	5
108-10-1	4-METHYL-2-PENTANONE	40	38.8	10		97	30	17
108-88-3	TOLUENE	10	10.7	1		107	20	2
10061-02-6	TRANS-1,3-DICHLOROPROPENE	10	11	1		110	20	7
79-00-5	1,1,2-TRICHLOROETHANE	10	10.8	1		108	20	10
591-78-6	2-HEXANONE	40	41	10		102	30	16
127-18-4	TETRACHLOROETHENE	10	11.1	1		111	20	2
142-28-9	1,3-DICHLOROPROPANE	10	10.3	1		103	20	5
124-48-1	DIBROMOCHLOROMETHANE	10	10.7	1		107	20	9
106-93-4	1,2-DIBROMOETHANE	10	10.5	1		105	20	10
544-10-5	1-CHLOROHEXANE	10	10.6	1		106	20	5
108-90-7	CHLOROBENZENE	10	10.8	1		108	20	0
630-20-6	1,1,1,2-TETRACHLOROETHANE	10	11	1		110	20	4
100-41-4	ETHYLBENZENE	10	10.8	1		108	20	3
136777-61-	M+P-XYLENE	20	21.7	1		109	20	2
95-47-6	O-XYLENE	10	10.9	1		109	20	3
100-42-5	STYRENE	10	11	1		110	20	1
75-25-2	BROMOFORM	10	10.4	1		104	20	9
98-82-8	ISOPROPYLBENZENE	10	10.9	1		109	20	3
96-18-4	1,2,3-TRICHLOROPROPANE	10	10.5	1		105	20	11
79-34-5	1,1,2,2-TETRACHLOROETHANE	10	10.2	1		102	20	4
108-86-1	BROMOBENZENE	10	10.6	1		106	20	0
103-65-1	N-PROPYLBENZENE	10	10.9	1		109	20	6
95-49-8	2-CHLOROTOLUENE	10	11.2	1		112	20	3

Data Package ID: VL0903157-1

Date Printed: Thursday, March 26, 2009

ALS Paragon

LIMS Version: 6.252A

Page 5 of 6

# GC/MS Volatiles

## Method SW8260\_25B

### Laboratory Control Sample and Laboratory Control Sample Duplicate

Lab Name: ALS Paragon

Work Order Number: 0903157

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204502

Lab ID: VL090323-3LCSD

Sample Matrix: WATER

% Moisture: N/A

Date Collected: N/A

Date Extracted: 03/23/2009

Date Analyzed: 03/23/2009

Prep Method: SW5030C

Prep Batch: VL090323-3

QCBatchID: VL090323-3-1

Run ID: VL090323-3A

Cleanup: NONE

Basis: N/A

File Name: C13946

Sample Aliquot: 10 ml

Final Volume: 10 ml

Result Units: UG/L

Clean DF: 1

CASNO	Target Analyte	Spike Added	LCSD Result	Reporting Limit	Result Qualifier	LCSD % Rec.	RPD Limit	RPD
108-67-8	1,3,5-TRIMETHYLBENZENE	10	11.2	1		112	20	4
106-43-4	4-CHLOROTOLUENE	10	10.9	1		109	20	4
98-06-6	TERT-BUTYLBENZENE	10	10.9	1		109	20	7
95-63-6	1,2,4-TRIMETHYLBENZENE	10	11.1	1		111	20	0
135-98-8	SEC-BUTYLBENZENE	10	10.8	1		108	20	5
541-73-1	1,3-DICHLOROBENZENE	10	10.8	1		108	20	3
99-87-6	P-ISOPROPYLTOLUENE	10	10.9	1		109	20	6
106-46-7	1,4-DICHLOROBENZENE	10	10.5	1		105	20	1
104-51-8	N-BUTYLBENZENE	10	11.2	1		112	20	6
95-50-1	1,2-DICHLOROBENZENE	10	10.7	1		107	20	2
96-12-8	1,2-DIBROMO-3-CHLOROPROPANE	10	10.3	2		103	20	9
120-82-1	1,2,4-TRICHLOROBENZENE	10	11	1		110	20	7
87-68-3	HEXACHLOROBUTADIENE	10	10.9	1		109	20	7
91-20-3	NAPHTHALENE	10	10.9	1		109	20	8
87-61-6	1,2,3-TRICHLOROBENZENE	10	10.8	1		108	20	5

### Surrogate Recovery LCS/LCSD

CASNO	Target Analyte	Spike Added	LCS % Rec.	LCS Flag	LCSD % Rec.	LCSD Flag	Control Limits
460-00-4	4-BROMOFLUOROBENZENE	25	104		99		78 - 129
1868-53-7	DIBROMOFLUOROMETHANE	25	100		98		80 - 124
2037-26-5	TOLUENE-D8	25	108		103		81 - 119

Data Package ID: VL0903157-1

Date Printed: Thursday, March 26, 2009

ALS Paragon

LIMS Version: 6.252A

Page 6 of 6

Data File : C:\HPCHEM\1\DATA\032309\C13948.D

Acq On : 23 Mar 2009 11:29

Sample : VL090323-3MB

Misc : 10mL un-heated purge

MS Integration Params: ettics.p

Quant Time: Mar 23 13:07 2009

Vial: 8

Operator: TWK-sop525r12

Inst : CSS Instr

Multiplr: 1.00

Quant Results File: 032209W.RES

Quant Method : C:\HPCHEM\1\METHODS\032209W.M (RTE Integrator)

Title : GC/MS Volatiles (S.O.P. 525)

Last Update : Mon Mar 23 13:04:42 2009

Response via : Initial Calibration

DataAcq Meth : 032209W

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene	9.34	96	1755067	25.00	ppb	0.00
53) Chlorobenzene-d5	12.48	82	654687	25.00	ppb	0.00
73) 1,4-Dichlorobenzene-d4	14.48	152	457889	25.00	ppb	0.00

## System Monitoring Compounds

34) Dibromofluoromethane	8.54	113	524111	24.91	ppb	0.00
Spiked Amount	25.000	Range	80 - 124	Recovery	=	99.64%
39) 1,2-dichloroethane-d4	9.01	65	393063	24.23	ppb	0.00
Spiked Amount	25.000	Range	62 - 139	Recovery	=	96.92%
54) Toluene-d8	11.03	98	1774712	26.03	ppb	0.00
Spiked Amount	25.000	Range	81 - 119	Recovery	=	104.12%
74) 4-Bromofluorobenzene	13.52	95	627374	26.29	ppb	0.00
Spiked Amount	25.000	Range	78 - 129	Recovery	=	105.16%

## Target Compounds

84) 1,2,4-Trimethylbenzene	14.17	105	12356	0.19	ppb	Qvalue # <del>N</del> 33
----------------------------	-------	-----	-------	------	-----	--------------------------


# Quantitation Report


Data File : C:\HPCHEM\1\DATA\032309\C13948.D  
 Acq On : 23 Mar 2009 11:29  
 Sample : VL090323-3MB  
 Misc : 10mL un-heated purge  
 MS Integration Params: ettics.p  
 Quant Time: Mar 23 13:07 2009

Vial: 8  
 Operator: TWK-sop525r12  
 Inst : CSS Instr  
 Multiplr: 1.00

Quant Results File: 032209W.RES


Method : C:\HPCHEM\1\METHODS\032209W.M (RTE Integrator)  
 Title : GC/MS Volatiles (S.O.P. 525)  
 Last Update : Mon Mar 23 13:04:42 2009  
 Response via : Initial Calibration

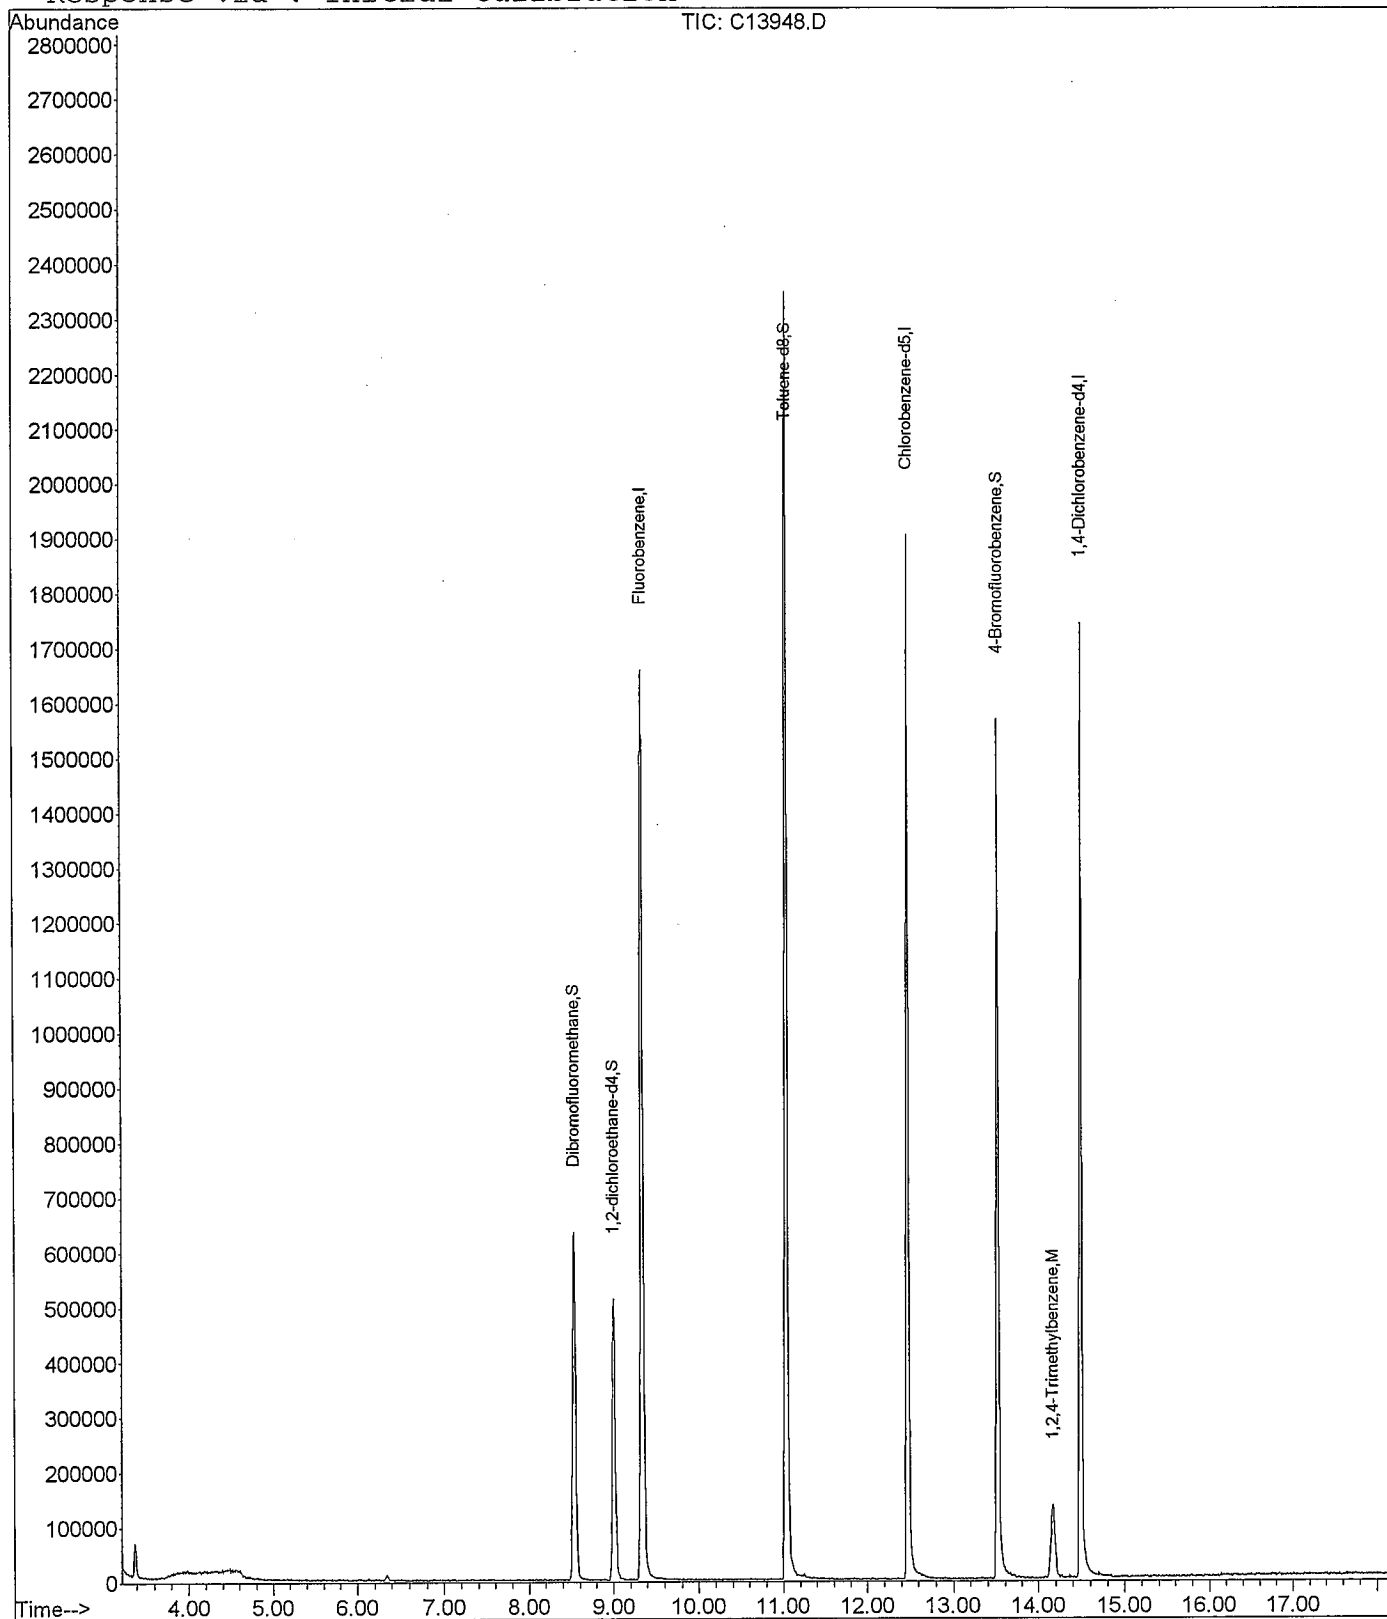

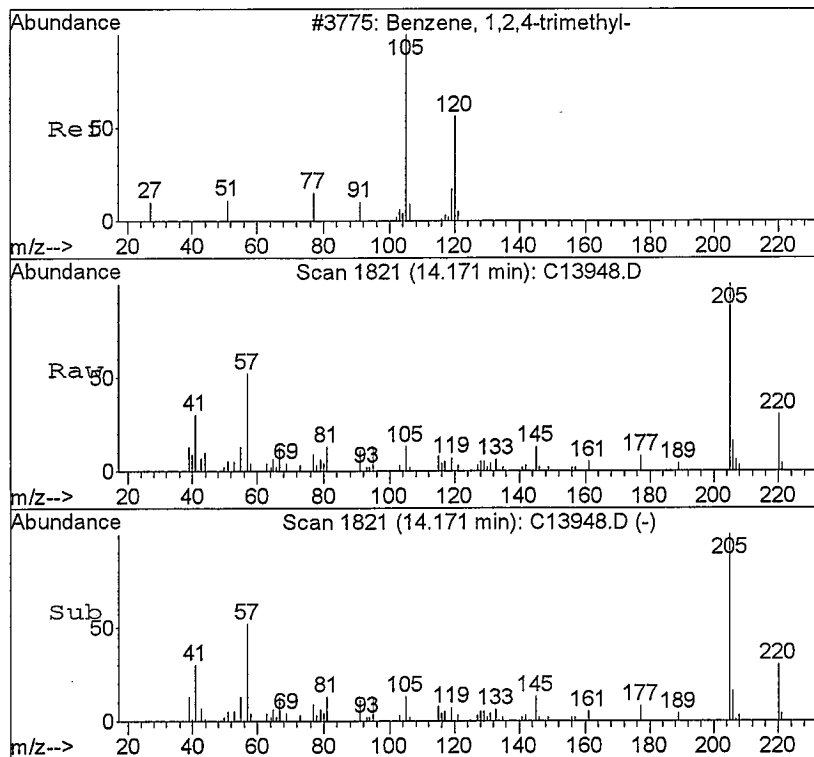

#84  
 1,2,4-Trimethylbenzene NO  
 Concen: 0.19 ppb  
 RT: 14.17 min Scan# 1821  
 Delta R.T. 0.04 min  
 Lab File: C13948.D  
 Acq: 23 Mar 2009 11:29

Tgt Ion: 105 Resp: 12356  
 Ion Ratio Lower Upper  
 105 100  
 120 0.0 25.6 59.8#

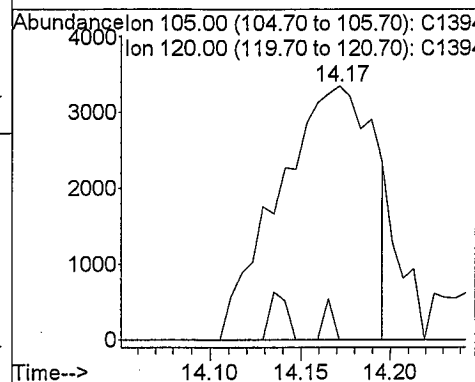

Butylated Hydroxytoluene carryover from Appendix 9 standard.  
 on 3/24/09

## Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\032309\C13948.D  
Acq On : 23 Mar 2009 11:29  
Sample : VL090323-3MB  
Misc : 10mL un-heated purge  
MS Integration Params: ettcs.p


Vial: 8  
Operator: TWK-sop525r12  
Inst : CSS Instr  
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\032209W.M (RTE Integrator)  
Title : GC/MS Volatiles (S.O.P. 525)  
Library : C:\DATABASE\NBS75K.L

\*\*\*\*\*  
Peak Number 1 Butylated Hydroxytoluene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.17	3.86 ppb	466599	1,4-Dichlorobenzene-d4	14.48

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		<u>Butylated Hydroxytoluene</u>	220	C15H24O	000128-37-0	94
2		Phenol, 2,6-bis(1,1-dimethylethyl)-	277	C17H27NO2	001918-11-2	53
3		5-Methyl-2-(N-methylphenylamino)-2-	206	C11H14N2S	029604-93-1	49
4		2H-1-Benzopyran, 6,7-dimethoxy-2,2-	220	C13H16O3	000644-06-4	45

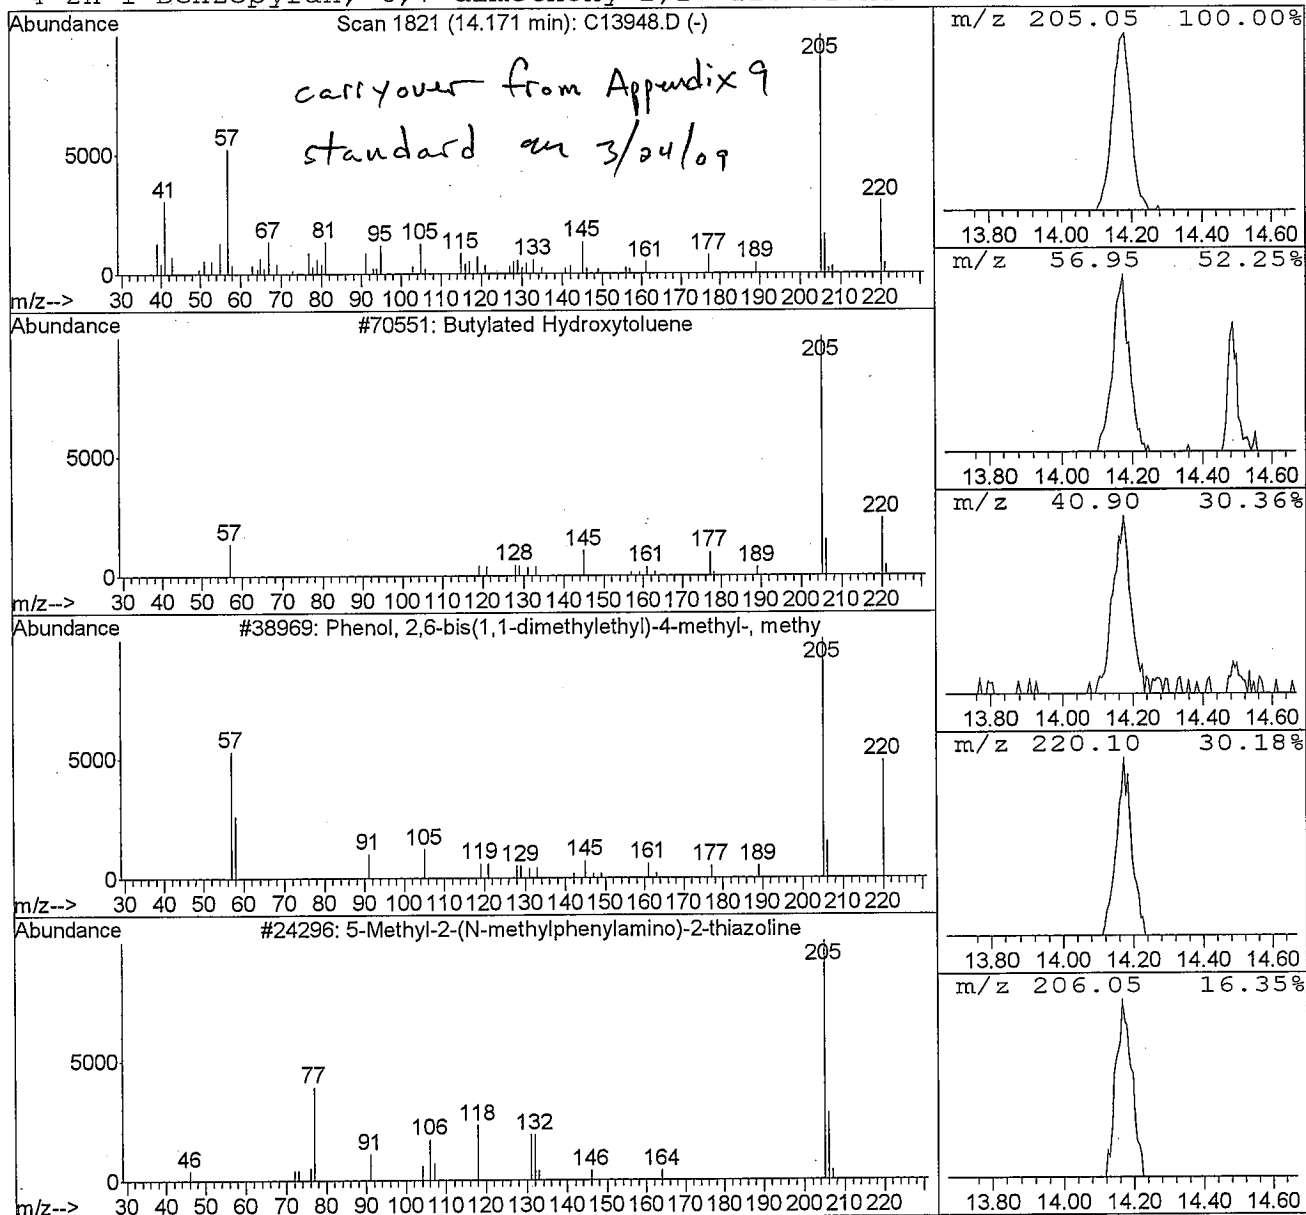



Data File : C:\HPCHEM\1\DATA\032309\C13955.D  
Acq On : 23 Mar 2009 14:20  
Sample : 0903157-1  
Misc : 10mL un-heated purge  
MS Integration Params: ettics.p  
Quant Time: Mar 23 14:51 2009

Vial: 15  
Operator: TWK-sop525r12  
Inst : CSS Instr  
Multiplr: 1.00

Quant Results File: 032209W.RES

Quant Method : C:\HPCHEM\1\METHODS\032209W.M (RTE Integrator)  
Title : GC/MS Volatiles (S.O.P. 525)  
Last Update : Mon Mar 23 13:04:42 2009  
Response via : Initial Calibration  
DataAcq Meth : 032209W

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene	9.34	96	1722764	25.00	ppb	0.00
53) Chlorobenzene-d5	12.48	82	651415	25.00	ppb	0.00
73) 1,4-Dichlorobenzene-d4	14.48	152	453845	25.00	ppb	0.00
System Monitoring Compounds						
34) Dibromofluoromethane	8.53	113	544658	26.37	ppb	0.00
Spiked Amount 25.000	Range 80 - 124		Recovery =	105.48%		
39) 1,2-dichloroethane-d4	9.00	65	391346	24.57	ppb	0.00
Spiked Amount 25.000	Range 62 - 139		Recovery =	98.28%		
54) Toluene-d8	11.03	98	1724483	25.42	ppb	0.00
Spiked Amount 25.000	Range 81 - 119		Recovery =	101.68%		
74) 4-Bromofluorobenzene	13.51	95	609631	25.77	ppb	0.00
Spiked Amount 25.000	Range 78 - 129		Recovery =	103.08%		
Target Compounds						
36) Cyclohexane	8.58	84	32285	1.08	ppb	Qvalue NTC93 TIC


# Quantitation Report


Data File : C:\HPCHEM\1\DATA\032309\C13955.D  
 Acq On : 23 Mar 2009 14:20  
 Sample : 0903157-1  
 Misc : 10mL un-heated purge  
 MS Integration Params: ettics.p  
 Quant Time: Mar 23 14:51 2009

Vial: 15  
 Operator: TWK-sop525r12  
 Inst : CSS Instr  
 Multiplr: 1.00

Quant Results File: 032209W.RES


Method : C:\HPCHEM\1\METHODS\032209W.M (RTE Integrator)  
 Title : GC/MS Volatiles (S.O.P. 525)  
 Last Update : Mon Mar 23 13:04:42 2009  
 Response via : Initial Calibration

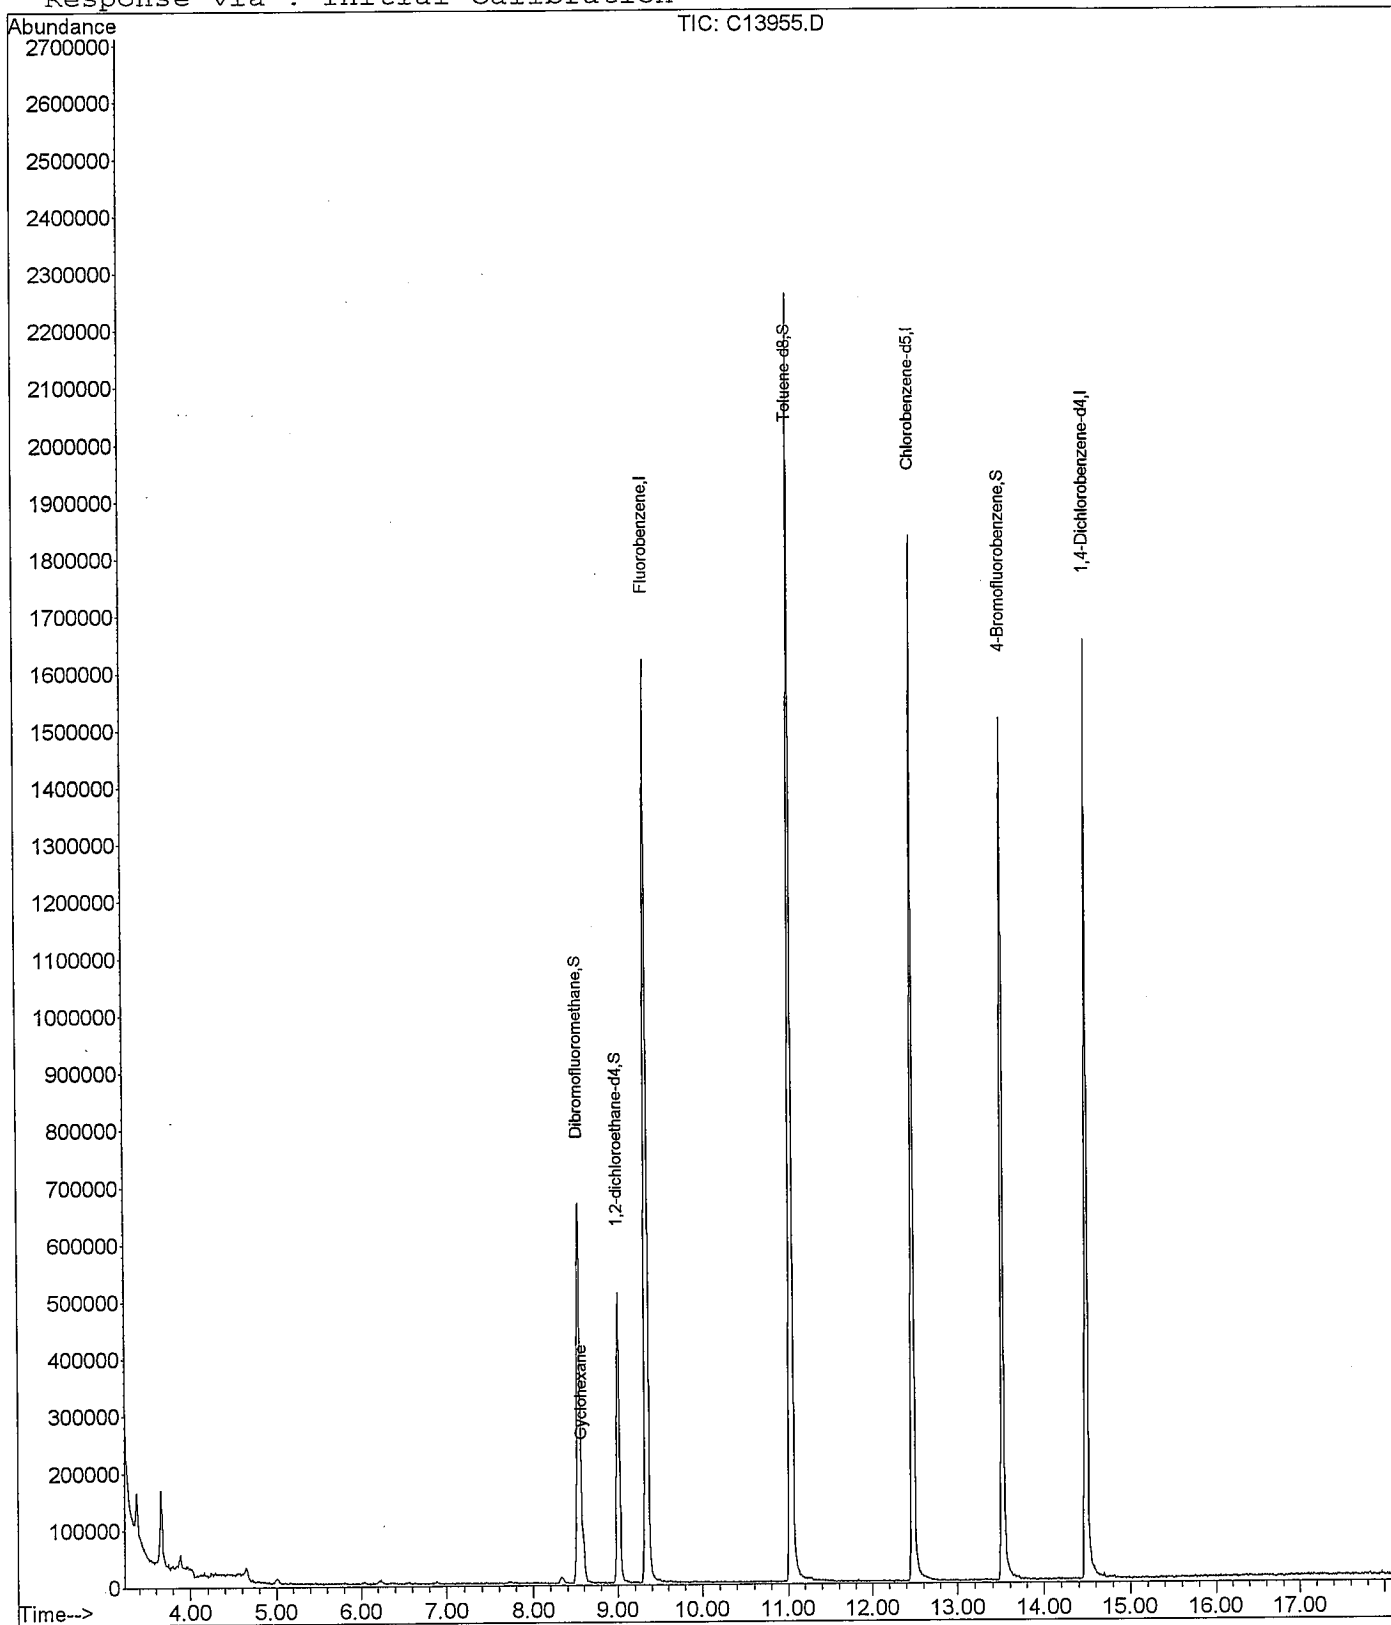

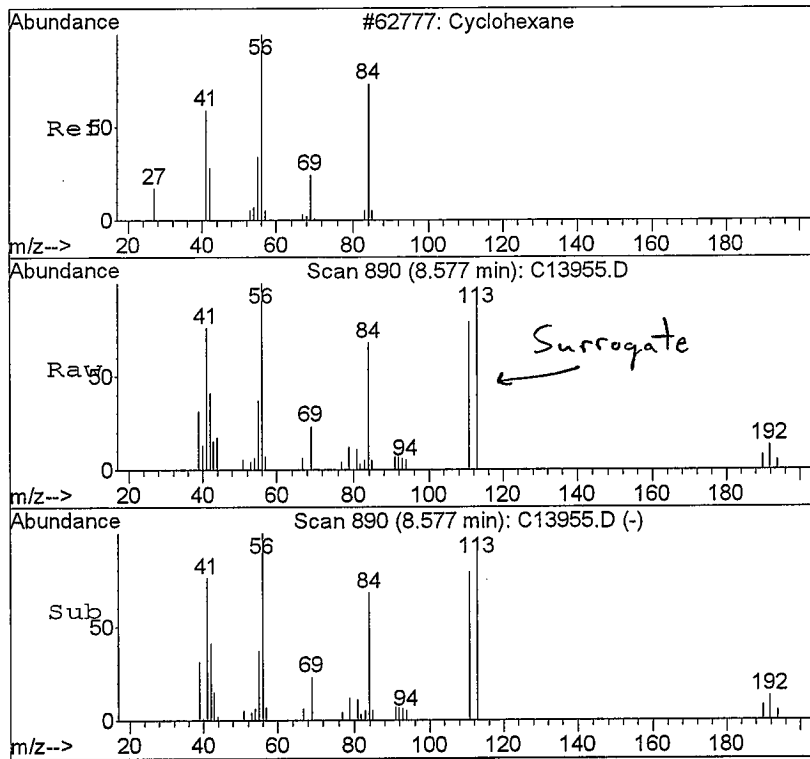

#36  
Cyclohexane  
Concen: 1.08 ppb  
RT: 8.58 min Scan# 890  
Delta R.T. -0.01 min  
Lab File: C13955.D  
Acq: 23 Mar 2009 14:20

Tgt Ion: 84 Resp: 32285  
Ion Ratio Lower Upper  
84 100  
41 111.4 78.5 117.7  
56 147.3 124.2 186.4  
55 55.1 43.8 65.6

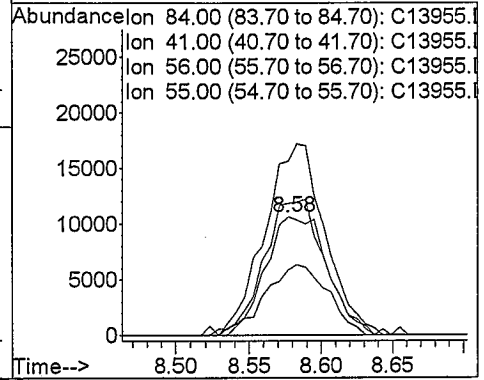

## Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\032309\C13955.D  
Acq On : 23 Mar 2009 14:20  
Sample : 0903157-1  
Misc : 10mL un-heated purge  
MS Integration Params: ettcs.p

Vial: 15  
Operator: TWK-sop525r12  
Inst : CSS Instr  
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\032209W.M (RTE Integrator)


Title : GC/MS Volatiles (S.O.P. 525)

Library : C:\DATABASE\NBS75K.L

\*\*\*\*\*  
Peak Number 1 Propane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.37	2.56 ppb	391902	Fluorobenzene	9.34

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane	44	C3H8	000074-98-6	64
2	2-Butenal, (E)-	70	C4H6O	000123-73-9	45
3	2-Butenal	70	C4H6O	004170-30-3	42
4	3-Butenoic acid	86	C4H6O2	000625-38-7	38

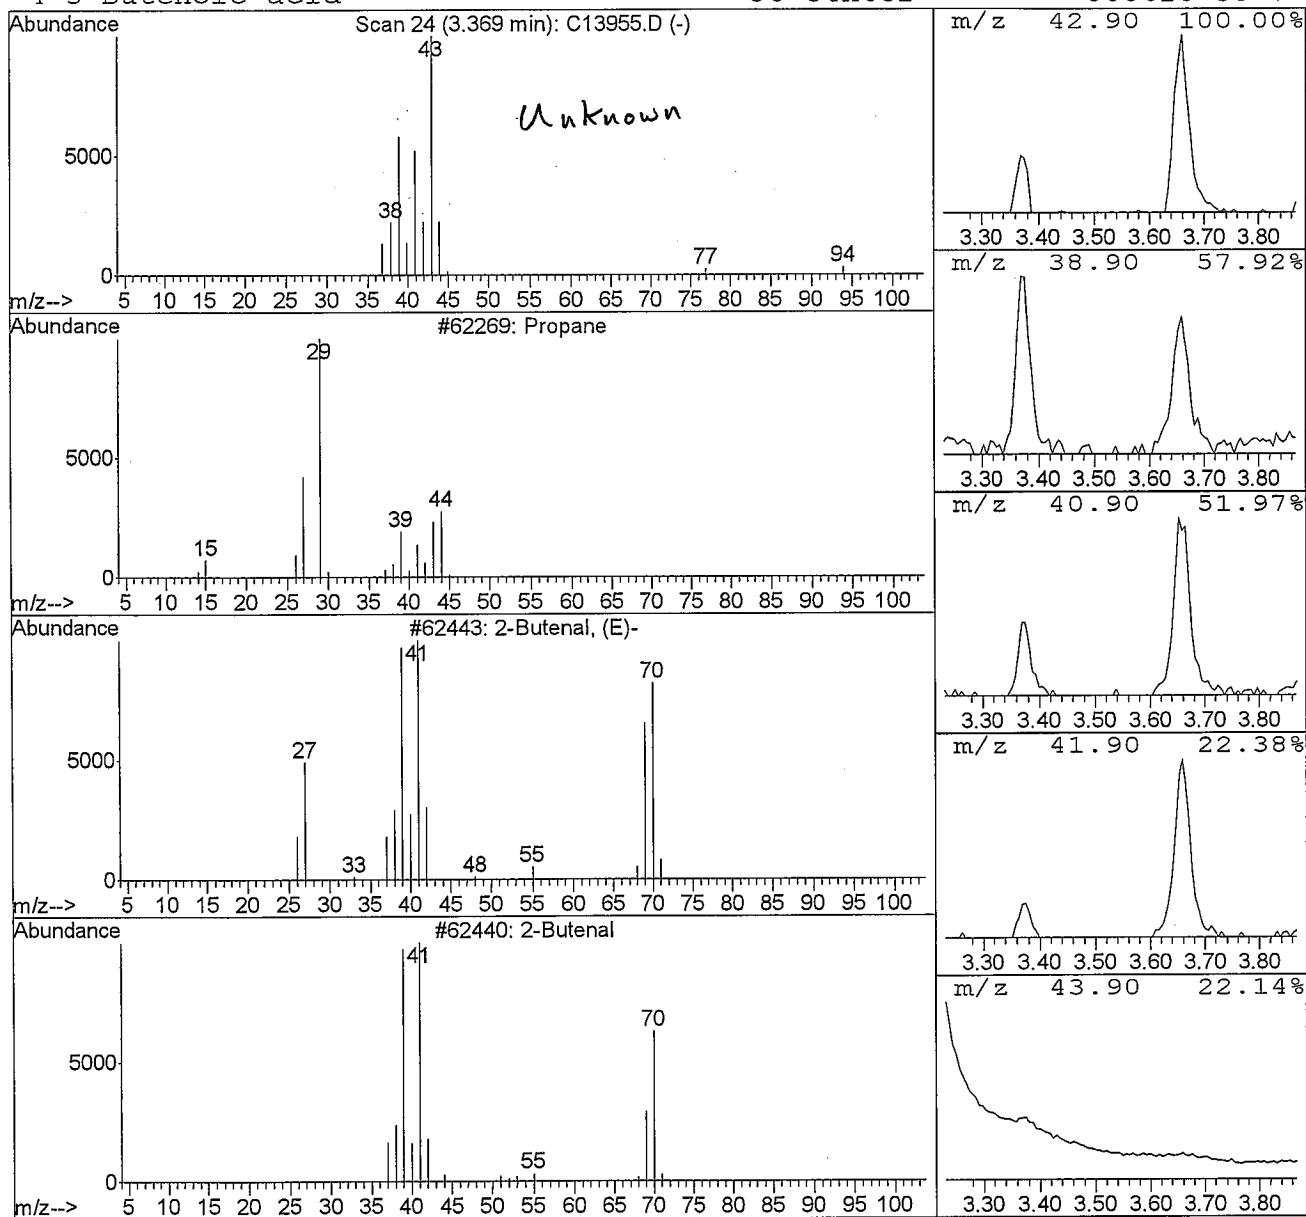

## Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\032309\C13955.D  
Acq On : 23 Mar 2009 14:20  
Sample : 0903157-1  
Misc : 10mL un-heated purge  
MS Integration Params: ettcs.p

Vial: 15  
Operator: TWK-sop525r12  
Inst : CSS Instr  
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\032209W.M (RTE Integrator)  
Title : GC/MS Volatiles (S.O.P. 525)  
Library : C:\DATABASE\NBS75K.L

\*\*\*\*\*  
Peak Number 1 1-Propanol, 2-methyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.66	1.79 ppb	273084	Fluorobenzene	9.34

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Propanol, 2-methyl-	74	C4H10O	000078-83-1	32
2			Isobutane	58	C4H10	000075-28-5	9
3			Propane	44	C3H8	000074-98-6	4
4			Propane, 1-chloro-2-methyl-	92	C4H9Cl	000513-36-0	4

