



# ALS Paragon



## GC/MS Semivolatiles Case Narrative

---

### Colorado Oil & Gas Conservation Commission

Complaint 200204503

Work Order Number: 0903158

1. This report consists of 1 water sample. The sample was received cool and intact by ALS Paragon on 03/20/09.
2. The sample was prepared and analyzed according to SW-846, 3rd Edition protocol utilizing SOP. Specifically, the water sample was extracted using continuous liquid-liquid extractors, according to SW-846 Method 3520C utilizing SOP 617 Revision 13.
3. The extracts were analyzed using GC/MS with a DB-5.625 capillary column according to SOP 506 Revision 15 based on SW-846 Method 8270D. All positive results were quantitated against the initial calibration standards using the internal standard technique. The identification of positive results was achieved by a comparison of the retention time and mass spectrum of the sample versus the daily calibration standard.
4. All initial calibration criteria for SPCC's and CCC's were met. If average response factors were used in the initial calibration, %RSD was  $\leq 15\%$ . If linear or higher order regression calibrations were used in the initial calibration, the coefficient of determination ( $r^2$ )  $\geq 0.99$ .
5. All initial calibration standards are verified by comparing a second source standard initial calibration verification (ICV) against the calibration curve. All target compounds in the second source verification had a %D of less than 25%.
6. All SPCC and CCC criteria were met in each of the daily (continuing) calibration verifications.
7. All method blank criteria were met.
8. All laboratory control sample and laboratory control sample duplicate recoveries and RPDs were within the acceptance criteria.
9. Since a sample from this order number was not the selected quality control (QC) sample, matrix specific QC results are not included in this report.



10. The sample was extracted and analyzed within the established holding time.
11. All surrogate recoveries were within acceptance criteria.
12. All internal standard recoveries were within acceptance criteria.

The data contained in the following report have been reviewed and approved by the personnel listed below. In addition, ALS Paragon certifies that the analyses reported herein are true, complete and correct within the limits of the methods employed.

SLJ

Sharon L. Jobes  
Organics Primary Data Reviewer

3/31-09

Date

Joe Hartman

Organics Final Data Reviewer

March 31, 2009

Date



**ALS Paragon**  
**Data Qualifier Flags**  
**Chromatography and Mass Spectrometry**

- U or ND:** This flag indicates that the compound was analyzed for but not detected.
- J:** This flag indicates an estimated value. This flag is used as follows: (1) when estimating a concentration for tentatively identified compounds (TICs) where a 1:1 response is assumed; (2) when the mass spectral and retention time data indicate the presence of a compound that meets the volatile and semivolatile GC/MS identification criteria, and the result is less than the reporting limit (RL) but greater than the method detection limit (MDL); (3) when the retention time data indicate the presence of a compound that meets the GC identification criteria, and the result is less than the RL but greater than the MDL; and (4) the reported value is estimated.
- B:** This flag is used when the analyte is detected in the associated method blank as well as in the sample. It indicates probable blank contamination and warns the data user. This flag shall be used for a tentatively identified compound (TIC) as well as for a positively identified target compound.
- E:** This flag identifies compounds whose concentration exceeds the upper level of the calibration range.
- A:** This flag indicates that a tentatively identified compound is a suspected aldol-condensation product.
- X:** This flag indicates that the analyte was diluted below an accurate quantitation level.
- \*:** This flag indicates that a spike recovery is equal to or outside the control criteria used.
- +:** This flag indicates that the relative percent difference (RPD) equals or exceeds the control criteria.

# ALS Paragon

## Sample Number(s) Cross-Reference Table

---

**Paragon OrderNum:** 0903158

**Client Name:** Colorado Oil & Gas Conservation Commission

**Client Project Name:** Complaint 200204503

**Client Project Number:**

**Client PO Number:** OE PHA 09000000004

---

Client Sample Number	Lab Sample Number	COC Number	Matrix	Date Collected	Time Collected
VanAlestyn 090319	0903158-1		WATER	19-Mar-09	12:40



**Paragon Analytics**  
A Division of DataChem Laboratories, Inc.

225 Commerce Drive Fort Collins, CO 80524  
800-443-1511 or (970) 490-1522 Fax

Accession Number (LAB ID) **0903158**

Originator: Retain pink copy!

Chain-of-Custody Date **3/19/09**

Page **1** of **1**

Project Name/No.: AFR	Sampler(s): C. Whitmore	Turnaround (circle one)		Standard	Rush (Due <b>14</b> )	(Dispose) Date <b>3/24</b>	or Return to Client
		1	2				
Report To: Peter Gintautas							
Phone: 719-846-3091							
Fax:							
E-mail: peter.gintautas@state.co.us							
Company: Col. Oil + Gas Enviro Chem.							
Address: 2425 E 2nd Street, Suite 100, Pueblo, CO 81004							
Comments: Quantitative analysis required							
Circle method (right); provide additional information as needed (comments).							
Sample ID	Date	Time *	Lab ID	Matrix	Preservative	No. of Containers	
Groundwater 39039	3/19/09	10:05	W	Water	(Indicate type... HCl, etc.)	10	
Pulsifer 09039	3/19/09	11:05	O	Oil		1	
VANASPIRA 09039	3/19/09	13:45	L	Gas		1	
ICASSYU 09039	3/19/09	13:45	S	Soil		1	
VOCs							
PCBs							
OC Pesticides							
Herbicides							
TCLP Organics SW1311							
TCLP Metals SW1311 Hg							
Total Metals by ICP Hg							
Dissolved Metals by ICP Hg							
Total Metals by ICP/MS							
Dissolved Metals by ICP/MS							
Inorganic Arsenic							
Solids:							
Total Dissolved Solids by TDS							
SW9040B SW9045C							
Gross Alpha / Beta							
Alpha-Emitting Radium							
Tritium							
Radium 226							
Radium 228							
Strontium 90 (Total Radionuclides)							
Gamma Isotopes							
Radon 222							
Radon 2222							
SM7510Rn							
Actinides by Paragon SOP							
Pu / U / Am / Th / Cm /							
SW9315 E903.0							
SW9320 E904.0							
E903.1							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							
Proton Radiation							
Gamma Radiation							
Alpha Radiation							
Neutron Radiation							
Electron Radiation							

## CONDITION OF SAMPLE UPON RECEIPT FORM

Paragon Analytics

Client: COGCC

Workorder No: 0903158

Project Manager: AW

Initials: LJO Date: 3/20/09

1. Does this project require any <b>special handling</b> in addition to standard Paragon procedures?	YES	NO	
2. Are custody <b>seals</b> on <b>shipping containers</b> intact?	NONE	YES	NO
3. Are Custody seals on <b>sample containers</b> intact?	<b>NONE</b>	YES	NO
4. Is there a <b>COC (Chain-of-Custody) present</b> or other representative documents?	YES	NO	
5. Are the <b>COC and bottle labels complete and legible?</b>	YES	NO	
6. Is the <b>COC in agreement</b> with samples received? (IDs, dates, times, no. of samples, no. of containers, matrix, requested analyses, etc.)	YES	NO	
7. Were <b>airbills / shipping documents</b> present and/or removable?	DROP OFF	YES	NO
8. Are all aqueous <b>samples requiring preservation preserved correctly?</b> (excluding volatiles)	N/A	YES	NO
9. Are all aqueous <b>non-preserved samples pH 4-9?</b>	N/A	YES	NO
10. Is there <b>sufficient sample</b> for the requested analyses?	YES	NO	
11. Were all samples placed in the <b>proper containers</b> for the requested analyses?	YES	NO	
12. Are all samples within <b>holding times</b> for the requested analyses?	YES	NO	
13. Were all sample containers received <b>intact?</b> (not broken or leaking, etc.)	YES	NO	
14. Are all samples requiring <b>no headspace</b> (VOC, GRO, RSK/MEE, Rx CN/S, radon) headspace free? <b>Size of bubble:</b> _____ < green pea _____ > green pea	N/A	YES	NO
15. Do perchlorate LCMS-MS samples <b>have headspace?</b> (at least 1/3 of container required)	N/A	YES	NO
16. Were samples checked for and free from the presence of <b>residual chlorine?</b> (Applicable when PM has indicated samples are from a chlorinated water source; note if field preservation with sodium thiosulfate was not observed.)	N/A	YES	NO
17. Were the samples <b>shipped on ice?</b>	YES	NO	
18. Were cooler temperatures measured at 0.1-6.0°C?	IR gun used*: #2	#4	RAD ONLY YES
Cooler #:	1		
Temperature (°C):	22		
No. of custody seals on cooler:	1		
External µR/hr reading:	13		
Background µR/hr reading:	11		
Were external µR/hr readings ≤ two times background and within DOT acceptance criteria? YES / NO / NA (If no. see Form 008.)			

**Additional Information:** PROVIDE DETAILS BELOW FOR A NO RESPONSE TO ANY QUESTION ABOVE, EXCEPT #1 AND #16.\* 3 of 18 40 ml vials for methane analysis listed no sample time on labels.  
3/20/09

• The 500ml poly for metals analysis needs to be filtered and preserved in house.

If applicable, was the client contacted? YES / NO / NA Contact: \_\_\_\_\_ Date/Time: \_\_\_\_\_

Project Manager Signature / Date: Carly 3/23/09

\*IR Gun #2: Oakton, SN 29922500201-0066

\*IR Gun #4: Oakton, SN 2372220101-0002

# GC/MS Semi-volatiles

## Method SW8270D

### Method Blank

Lab Name: ALS Paragon

Work Order Number: 0903158

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204503

Lab ID: EX090324-2MB

Sample Matrix: WATER

% Moisture: N/A

Date Collected: N/A

Date Extracted: 24-Mar-09

Date Analyzed: 28-Mar-09

Prep Method: SW3520 Rev C

Prep Batch: EX090324-2

QCBatchID: EX090324-2-1

Run ID: SV090328-1

Cleanup: NONE

Basis: N/A

File Name: N5703

Sample Aliquot: 1000 ml

Final Volume: 1 ml

Result Units: UG/L

Clean DF: 1

CASNO	Target Analyte	DF	Result	Reporting Limit	Result Qualifier	EPA Qualifier
110-86-1	PYRIDINE	1	10	10	U	
62-75-9	N-NITROSODIMETHYLAMINE	1	10	10	U	
62-53-3	ANILINE	1	10	10	U	
108-95-2	PHENOL	1	10	10	U	
111-44-4	BIS(2-CHLOROETHYL)ETHER	1	10	10	U	
95-57-8	2-CHLOROPHENOL	1	10	10	U	
541-73-1	1,3-DICHLOROBENZENE	1	10	10	U	
106-46-7	1,4-DICHLOROBENZENE	1	10	10	U	
95-50-1	1,2-DICHLOROBENZENE	1	10	10	U	
100-51-6	BENZYL ALCOHOL	1	10	10	U	
108-60-1	BIS(2-CHLOROISOPROPYL)ETHER	1	10	10	U	
95-48-7	2-METHYLPHENOL	1	10	10	U	
621-64-7	N-NITROSO-DI-N-PROPYLAMINE	1	10	10	U	
108-39-4	3+4-METHYLPHENOL	1	10	10	U	
67-72-1	HEXACHLOROETHANE	1	10	10	U	
98-95-3	NITROBENZENE	1	10	10	U	
78-59-1	ISOPHORONE	1	10	10	U	
88-75-5	2-NITROPHENOL	1	10	10	U	
105-67-9	2,4-DIMETHYLPHENOL	1	10	10	U	
111-91-1	BIS(2-CHLOROETHOXY)METHANE	1	10	10	U	
120-83-2	2,4-DICHLOROPHENOL	1	10	10	U	
65-85-0	BENZOIC ACID	1	50	50	U	
120-82-1	1,2,4-TRICHLOROBENZENE	1	10	10	U	
91-20-3	NAPHTHALENE	1	10	10	U	
106-47-8	4-CHLOROANILINE	1	10	10	U	
87-68-3	HEXACHLOROBUTADIENE	1	10	10	U	
59-50-7	4-CHLORO-3-METHYLPHENOL	1	10	10	U	

Data Package ID: SV0903158-1

Date Printed: Tuesday, March 31, 2009

ALS Paragon

LIMS Version: 6.253A

Page 1 of 3

# GC/MS Semi-volatiles

## Method SW8270D

### Method Blank

Lab Name: ALS Paragon

Work Order Number: 0903158

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204503

Lab ID: EX090324-2MB

Sample Matrix: WATER

% Moisture: N/A

Date Collected: N/A

Date Extracted: 24-Mar-09

Date Analyzed: 28-Mar-09

Prep Method: SW3520 Rev C

Prep Batch: EX090324-2

QCBatchID: EX090324-2-1

Run ID: SV090328-1

Cleanup: NONE

Basis: N/A

File Name: N5703

Sample Aliquot: 1000 ml

Final Volume: 1 ml

Result Units: UG/L

Clean DF: 1

91-57-6	2-METHYLNAPHTHALENE	1	10	10	U	
90-12-0	1-METHYLNAPHTHALENE	1	10	10	U	
77-47-4	HEXACHLOROCYCLOPENTADIENE	1	10	10	U	
88-06-2	2,4,6-TRICHLOROPHENOL	1	10	10	U	
95-95-4	2,4,5-TRICHLOROPHENOL	1	10	10	U	
91-58-7	2-CHLORONAPHTHALENE	1	10	10	U	
88-74-4	2-NITROANILINE	1	20	20	U	
131-11-3	DIMETHYL PHTHALATE	1	10	10	U	
606-20-2	2,6-DINITROTOLUENE	1	10	10	U	
208-96-8	ACENAPHTHYLENE	1	10	10	U	
99-09-2	3-NITROANILINE	1	20	20	U	
83-32-9	ACENAPHTHENE	1	10	10	U	
51-28-5	2,4-DINITROPHENOL	1	20	20	U	
100-02-7	4-NITROPHENOL	1	20	20	U	
132-64-9	DIBENZOFURAN	1	10	10	U	
121-14-2	2,4-DINITROTOLUENE	1	10	10	U	
84-66-2	DIETHYL PHTHALATE	1	10	10	U	
86-73-7	FLUORENE	1	10	10	U	
7005-72-3	4-CHLOROPHENYL PHENYL ETHER	1	10	10	U	
100-01-6	4-NITROANILINE	1	20	20	U	
103-33-3	AZOBENZENE	1	10	10	U	
534-52-1	4,6-DINITRO-2-METHYLPHENOL	1	20	20	U	
86-30-6	N-NITROSODIPHENYLAMINE	1	10	10	U	
101-55-3	4-BROMOPHENYL PHENYL ETHER	1	10	10	U	
118-74-1	HEXACHLOROBENZENE	1	10	10	U	
58-90-2	2,3,4,6-TETRACHLOROPHENOL	1	10	10	U	
87-86-5	PENTACHLOROPHENOL	1	20	20	U	
85-01-8	PHENANTHRENE	1	10	10	U	
120-12-7	ANTHRACENE	1	10	10	U	

Data Package ID: SV0903158-1

Date Printed: Tuesday, March 31, 2009

ALS Paragon

LIMS Version: 6.253A

Page 2 of 3

# GC/MS Semi-volatiles

## Method SW8270D

### Method Blank

Lab Name: ALS Paragon

Work Order Number: 0903158

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204503

Lab ID: EX090324-2MB

Sample Matrix: WATER

% Moisture: N/A

Date Collected: N/A

Date Extracted: 24-Mar-09

Date Analyzed: 28-Mar-09

Prep Method: SW3520 Rev C

Prep Batch: EX090324-2

QCBatchID: EX090324-2-1

Run ID: SV090328-1

Cleanup: NONE

Basis: N/A

File Name: N5703

Sample Aliquot: 1000 ml

Final Volume: 1 ml

Result Units: UG/L

Clean DF: 1

86-74-8	CARBAZOLE	1	10	10	U	
84-74-2	DI-N-BUTYL PHTHALATE	1	10	10	U	
206-44-0	FLUORANTHENE	1	10	10	U	
129-00-0	PYRENE	1	10	10	U	
85-68-7	BUTYL BENZYL PHTHALATE	1	10	10	U	
56-55-3	BENZO(A)ANTHRACENE	1	10	10	U	
91-94-1	3,3'-DICHLOROBENZIDINE	1	10	10	U	
218-01-9	CHRYSENE	1	10	10	U	
117-81-7	BIS(2-ETHYLHEXYL)PHTHALATE	1	10	10	U	
117-84-0	DI-N-OCTYL PHTHALATE	1	10	10	U	
205-99-2	BENZO(B)FLUORANTHENE	1	10	10	U	
207-08-9	BENZO(K)FLUORANTHENE	1	10	10	U	
50-32-8	BENZO(A)PYRENE	1	10	10	U	
193-39-5	INDENO(1,2,3-CD)PYRENE	1	10	10	U	
53-70-3	DIBENZO(A,H)ANTHRACENE	1	10	10	U	
191-24-2	BENZO(G,H,I)PERYLENE	1	10	10	U	

### Surrogate Recovery

CASNO	Surrogate Analyte	Result	Flag	Spike Amount	Percent Recovery	Control Limits
118-79-6	2,4,6-TRIBROMOPHENOL	49.9		75	67	23 - 100
321-60-8	2-FLUOROBIPHENYL	45.4		50	91	21 - 106
367-12-4	2-FLUOROPHENOL	70.7		75	94	21 - 100
4165-60-0	NITROBENZENE-D5	47		50	94	34 - 111
4165-62-2	PHENOL-D5	71.6		75	96	15 - 104
1718-51-0	TERPHENYL-D14	51		50	102	33 - 111

Data Package ID: SV0903158-1

Date Printed: Tuesday, March 31, 2009

ALS Paragon

LIMS Version: 6.253A

Page 3 of 3

# GC/MS Semi-volatiles

## Method SW8270

### Tentatively Identified Compounds

Lab Name: ALS Paragon

Work Order Number: 0903158

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204503

Field ID:   
Lab ID: EX090324-2MB

Sample Matrix: WATER

% Moisture: N/A

Date Collected: N/A

Date Extracted: 24-Mar-09

Date Analyzed: 28-Mar-09

Prep Batch: EX090324-2

QCBatchID: EX090324-2-1

Run ID: SV090328-1

Cleanup: NONE

Basis: As Received

Sample Aliquot: 1000 ml

Final Volume: 1 ml

Clean DF: 1

File Name: N5703

CASNO	Retention Time	Target Analyte	Dilution Factor	Result	Units	Qualifier
	3.91	OXYGENATED HYDROCARBON1	1	11	UG/L	J

Data Package ID: SV0903158-1

Date Printed: Tuesday, March 31, 2009

ALS Paragon

LIMS Version: 6.253A

Page 2 of 2

# GC/MS Semi-volatiles

## Method SW8270D Sample Results

Lab Name: ALS Paragon

Work Order Number: 0903158

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204503

Field ID: VanAlestyn 090319	Sample Matrix: WATER	Prep Batch: EX090324-2	Sample Aliquot: 1065 ml
Lab ID: 0903158-1	% Moisture: N/A	QCBatchID: EX090324-2-1	Final Volume: 1 ml
	Date Collected: 19-Mar-09	Run ID: SV090328-1	Result Units: UG/L
	Date Extracted: 24-Mar-09	Cleanup: NONE	Clean DF: 1
	Date Analyzed: 28-Mar-09	Basis: As Received	
	Prep Method: SW3520 Rev C	File Name: N5708	

CASNO	Target Analyte	Dilution Factor	Result	Reporting Limit	Result Qualifier	EPA Qualifier
110-86-1	PYRIDINE	1	9.4	9.4	U	
62-75-9	N-NITROSODIMETHYLAMINE	1	9.4	9.4	U	
62-53-3	ANILINE	1	9.4	9.4	U	
108-95-2	PHENOL	1	9.4	9.4	U	
111-44-4	BIS(2-CHLOROETHYL)ETHER	1	9.4	9.4	U	
95-57-8	2-CHLOROPHENOL	1	9.4	9.4	U	
541-73-1	1,3-DICHLOROBENZENE	1	9.4	9.4	U	
106-46-7	1,4-DICHLOROBENZENE	1	9.4	9.4	U	
95-50-1	1,2-DICHLOROBENZENE	1	9.4	9.4	U	
100-51-6	BENZYL ALCOHOL	1	9.4	9.4	U	
108-60-1	BIS(2-CHLOROISOPROPYL)ETHER	1	9.4	9.4	U	
95-48-7	2-METHYLPHENOL	1	9.4	9.4	U	
621-64-7	N-NITROSO-DI-N-PROPYLAMINE	1	9.4	9.4	U	
108-39-4	3+4-METHYLPHENOL	1	9.4	9.4	U	
67-72-1	HEXACHLOROETHANE	1	9.4	9.4	U	
98-95-3	NITROBENZENE	1	9.4	9.4	U	
78-59-1	ISOPHORONE	1	9.4	9.4	U	
88-75-5	2-NITROPHENOL	1	9.4	9.4	U	
105-67-9	2,4-DIMETHYLPHENOL	1	9.4	9.4	U	
111-91-1	BIS(2-CHLOROETHOXY)METHANE	1	9.4	9.4	U	
120-83-2	2,4-DICHLOROPHENOL	1	9.4	9.4	U	
65-85-0	BENZOIC ACID	1	47	47	U	
120-82-1	1,2,4-TRICHLOROBENZENE	1	9.4	9.4	U	
91-20-3	NAPHTHALENE	1	9.4	9.4	U	
106-47-8	4-CHLOROANILINE	1	9.4	9.4	U	
87-68-3	HEXACHLOROBUTADIENE	1	9.4	9.4	U	
59-50-7	4-CHLORO-3-METHYLPHENOL	1	9.4	9.4	U	

Data Package ID: SV0903158-1

Date Printed: Tuesday, March 31, 2009

ALS Paragon

LIMS Version: 6.253A

Page 1 of 3

# GC/MS Semi-volatiles

## Method SW8270D Sample Results

Lab Name: ALS Paragon

Work Order Number: 0903158

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204503

Field ID:	VanAlestyn 090319
Lab ID:	0903158-1

Sample Matrix: WATER  
% Moisture: N/A  
Date Collected: 19-Mar-09  
Date Extracted: 24-Mar-09  
Date Analyzed: 28-Mar-09  
Prep Method: SW3520 Rev C

Prep Batch: EX090324-2  
QCBatchID: EX090324-2-1  
Run ID: SV090328-1  
Cleanup: NONE  
Basis: As Received  
File Name: N5708

Sample Aliquot: 1065 ml  
Final Volume: 1 ml  
Result Units: UG/L  
Clean DF: 1

91-57-6	2-METHYLNAPHTHALENE	1	9.4	9.4	U	
90-12-0	1-METHYLNAPHTHALENE	1	9.4	9.4	U	
77-47-4	HEXACHLOROCYCLOPENTADIENE	1	9.4	9.4	U	
88-06-2	2,4,6-TRICHLOROPHENOL	1	9.4	9.4	U	
95-95-4	2,4,5-TRICHLOROPHENOL	1	9.4	9.4	U	
91-58-7	2-CHLORONAPHTHALENE	1	9.4	9.4	U	
88-74-4	2-NITROANILINE	1	19	19	U	
131-11-3	DIMETHYL PHTHALATE	1	9.4	9.4	U	
606-20-2	2,6-DINITROTOLUENE	1	9.4	9.4	U	
208-96-8	ACENAPHTHYLENE	1	9.4	9.4	U	
99-09-2	3-NITROANILINE	1	19	19	U	
83-32-9	ACENAPHTHENE	1	9.4	9.4	U	
51-28-5	2,4-DINITROPHENOL	1	19	19	U	
100-02-7	4-NITROPHENOL	1	19	19	U	
132-64-9	DIBENZOFURAN	1	9.4	9.4	U	
121-14-2	2,4-DINITROTOLUENE	1	9.4	9.4	U	
84-66-2	DIETHYL PHTHALATE	1	9.4	9.4	U	
86-73-7	FLUORENE	1	9.4	9.4	U	
7005-72-3	4-CHLOROPHENYL PHENYL ETHER	1	9.4	9.4	U	
100-01-6	4-NITROANILINE	1	19	19	U	
103-33-3	AZOBENZENE	1	9.4	9.4	U	
534-52-1	4,6-DINITRO-2-METHYLPHENOL	1	19	19	U	
86-30-6	N-NITROSODIPHENYLAMINE	1	9.4	9.4	U	
101-55-3	4-BROMOPHENYL PHENYL ETHER	1	9.4	9.4	U	
118-74-1	HEXACHLOROBENZENE	1	9.4	9.4	U	
58-90-2	2,3,4,6-TETRACHLOROPHENOL	1	9.4	9.4	U	
87-86-5	PENTACHLOROPHENOL	1	19	19	U	
85-01-8	PHENANTHRENE	1	9.4	9.4	U	
120-12-7	ANTHRACENE	1	9.4	9.4	U	

Data Package ID: SV0903158-1

Date Printed: Tuesday, March 31, 2009

ALS Paragon

LIMS Version: 6.253A

Page 2 of 3

# GC/MS Semi-volatiles

## Method SW8270D Sample Results

Lab Name: ALS Paragon

Work Order Number: 0903158

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204503

Field ID:	VanAlestyn 090319
Lab ID:	0903158-1

Sample Matrix: WATER  
% Moisture: N/A  
Date Collected: 19-Mar-09  
Date Extracted: 24-Mar-09  
Date Analyzed: 28-Mar-09  
Prep Method: SW3520 Rev C

Prep Batch: EX090324-2  
QCBatchID: EX090324-2-1  
Run ID: SV090328-1  
Cleanup: NONE  
Basis: As Received  
File Name: N5708

Sample Aliquot: 1065 ml  
Final Volume: 1 ml  
Result Units: UG/L  
Clean DF: 1

86-74-8	CARBAZOLE	1	9.4	9.4	U	
84-74-2	DI-N-BUTYL PHTHALATE	1	9.4	9.4	U	
206-44-0	FLUORANTHENE	1	9.4	9.4	U	
129-00-0	PYRENE	1	9.4	9.4	U	
85-68-7	BUTYL BENZYL PHTHALATE	1	9.4	9.4	U	
56-55-3	BENZO(A)ANTHRACENE	1	9.4	9.4	U	
91-94-1	3,3'-DICHLOROBENZIDINE	1	9.4	9.4	U	
218-01-9	CHRYSENE	1	9.4	9.4	U	
117-81-7	BIS(2-ETHYLHEXYL)PHTHALATE	1	9.4	9.4	U	
117-84-0	DI-N-OCTYL PHTHALATE	1	9.4	9.4	U	
205-99-2	BENZO(B)FLUORANTHENE	1	9.4	9.4	U	
207-08-9	BENZO(K)FLUORANTHENE	1	9.4	9.4	U	
50-32-8	BENZO(A)PYRENE	1	9.4	9.4	U	
193-39-5	INDENO(1,2,3-CD)PYRENE	1	9.4	9.4	U	
53-70-3	DIBENZO(A,H)ANTHRACENE	1	9.4	9.4	U	
191-24-2	BENZO(G,H,I)PERYLENE	1	9.4	9.4	U	

## Surrogate Recovery

CASNO	Surrogate Analyte	Result	Flag	Spike Amount	Percent Recovery	Control Limits
118-79-6	2,4,6-TRIBROMOPHENOL	46.2		70.4	66	23 - 100
321-60-8	2-FLUOROBIPHENYL	40.8		46.9	87	21 - 106
367-12-4	2-FLUOROPHENOL	58.9		70.4	84	21 - 100
4165-60-0	NITROBENZENE-D5	40.2		46.9	86	34 - 111
4165-62-2	PHENOL-D5	61.1		70.4	87	15 - 104
1718-51-0	TERPHENYL-D14	44.2		46.9	94	33 - 111

Data Package ID: SV0903158-1

Date Printed: Tuesday, March 31, 2009

ALS Paragon

LIMS Version: 6.253A

Page 3 of 3

# GC/MS Semi-volatiles

## Method SW8270

### Tentatively Identified Compounds

Lab Name: ALS Paragon

Work Order Number: 0903158

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204503

Field ID:	VanAlestyn 090319
Lab ID:	0903158-1

Sample Matrix: WATER

% Moisture: N/A

Date Collected: 19-Mar-09

Date Extracted: 24-Mar-09

Date Analyzed: 28-Mar-09

Prep Batch: EX090324-2

QCBatchID: EX090324-2-1

Run ID: SV090328-1

Cleanup: NONE

Basis: As Received

Sample Aliquot: 1065 ml

Final Volume: 1 ml

Clean DF: 1

File Name: N5708

CASNO	Retention Time	Target Analyte	Dilution Factor	Result	Units	Qualifier
	3.91	OXYGENATED HYDROCARBON1	1	18	UG/L	B,J

Data Package ID: SV0903158-1

Date Printed: Tuesday, March 31, 2009

ALS Paragon

LIMS Version: 6.253A

Page 1 of 2

# GC/MS Semi-volatiles

## Method SW8270D

### Laboratory Control Sample and Laboratory Control Sample Duplicate

Lab Name: ALS Paragon

Work Order Number: 0903158

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204503

Lab ID: EX090324-2LCS	Sample Matrix: WATER % Moisture: N/A Date Collected: N/A Date Extracted: 03/24/2009 Date Analyzed: 03/28/2009 Prep Method: SW3520C	Prep Batch: EX090324-2 QCBatchID: EX090324-2-1 Run ID: SV090328-1 Cleanup: NONE Basis: N/A File Name: N5704	Sample Aliquot: 1000 ml Final Volume: 1 ml Result Units: UG/L Clean DF: 1
-----------------------	---	--	--

CASNO	Target Analyte	Spike Added	LCS Result	Reporting Limit	Result Qualifier	LCS % Rec.	Control Limits
110-86-1	PYRIDINE	60	42	10		70	10 - 108%
62-75-9	N-NITROSODIMETHYLAMINE	60	53.5	10		89	26 - 110%
62-53-3	ANILINE	60	50.3	10		84	25 - 125%
108-95-2	PHENOL	60	52	10		87	49 - 101%
111-44-4	BIS(2-CHLOROETHYL)ETHER	60	51.9	10		86	37 - 110%
95-57-8	2-CHLOROPHENOL	60	49.9	10		83	37 - 106%
541-73-1	1,3-DICHLOROBENZENE	60	45.9	10		76	32 - 98%
106-46-7	1,4-DICHLOROBENZENE	60	46.1	10		77	32 - 98%
95-50-1	1,2-DICHLOROBENZENE	60	46.9	10		78	33 - 102%
100-51-6	BENZYL ALCOHOL	60	53	10		88	30 - 112%
108-60-1	BIS(2-CHLOROISOPROPYL)ETHER	60	50.1	10		83	26 - 131%
95-48-7	2-METHYLPHENOL	60	50.6	10		84	38 - 109%
621-64-7	N-NITROSO-DI-N-PROPYLAMINE	60	52.1	10		87	34 - 128%
108-39-4	3+4-METHYLPHENOL	60	49.3	10		82	32 - 110%
67-72-1	HEXACHLOROETHANE	60	45.3	10		76	28 - 94%
98-95-3	NITROBENZENE	60	32.2	10		54	44 - 109%
78-59-1	ISOPHORONE	60	45.7	10		76	50 - 112%
88-75-5	2-NITROPHENOL	60	44.4	10		74	39 - 113%
105-67-9	2,4-DIMETHYLPHENOL	60	42.1	10		70	28 - 109%
111-91-1	BIS(2-CHLOROETHOXY)METHANE	60	45.9	10		76	46 - 107%
120-83-2	2,4-DICHLOROPHENOL	60	45	10		75	48 - 105%
65-85-0	BENZOIC ACID	100	41.9	50	J	42	10 - 125%
120-82-1	1,2,4-TRICHLOROBENZENE	60	39.6	10		66	37 - 107%
91-20-3	NAPHTHALENE	60	43.5	10		72	39 - 102%
106-47-8	4-CHLOROANILINE	60	45.2	10		75	15 - 109%
87-68-3	HEXACHLOROBUTADIENE	60	37.7	10		63	27 - 103%

Data Package ID: SV0903158-1

Date Printed: Tuesday, March 31, 2009

ALS Paragon

LIMS Version: 6.253A

Page 1 of 7

# GC/MS Semi-volatiles

## Method SW8270D

### Laboratory Control Sample and Laboratory Control Sample Duplicate

Lab Name: ALS Paragon

Work Order Number: 0903158

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204503

Lab ID: EX090324-2LCS	Sample Matrix: WATER % Moisture: N/A Date Collected: N/A Date Extracted: 03/24/2009 Date Analyzed: 03/28/2009 Prep Method: SW3520C	Prep Batch: EX090324-2 QCBatchID: EX090324-2-1 Run ID: SV090328-1 Cleanup: NONE Basis: N/A File Name: N5704	Sample Aliquot: 1000 ml Final Volume: 1 ml Result Units: UG/L Clean DF: 1
-----------------------	---	--	--

CASNO	Target Analyte	Spike Added	LCS Result	Reporting Limit	Result Qualifier	LCS % Rec.	Control Limits
59-50-7	4-CHLORO-3-METHYLPHENOL	60	48.6	10		81	47 - 111%
91-57-6	2-METHYLNAPHTHALENE	60	43.3	10		72	46 - 104%
90-12-0	1-METHYLNAPHTHALENE	60	49.7	10		83	46 - 104%
77-47-4	HEXACHLOROCYCLOPENTADIENE	60	13.8	10		23	10 - 125%
88-06-2	2,4,6-TRICHLOROPHENOL	60	51.6	10		86	49 - 113%
95-95-4	2,4,5-TRICHLOROPHENOL	60	54.5	10		91	49 - 111%
91-58-7	2-CHLORONAPHTHALENE	60	50.3	10		84	36 - 137%
88-74-4	2-NITROANILINE	60	59.7	20		99	48 - 115%
131-11-3	DIMETHYL PHTHALATE	60	53.7	10		89	25 - 127%
606-20-2	2,6-DINITROTOLUENE	60	56.4	10		94	49 - 117%
208-96-8	ACENAPHTHYLENE	60	53.6	10		89	50 - 107%
99-09-2	3-NITROANILINE	60	58.2	20		97	19 - 126%
83-32-9	ACENAPHTHENE	60	53	10		88	47 - 108%
51-28-5	2,4-DINITROPHENOL	60	51.3	20		86	14 - 138%
100-02-7	4-NITROPHENOL	60	52	20		87	21 - 119%
132-64-9	DIBENZOFURAN	60	53	10		88	54 - 107%
121-14-2	2,4-DINITROTOLUENE	60	54.5	10		91	51 - 118%
84-66-2	DIETHYL PHTHALATE	60	56.3	10		94	41 - 118%
86-73-7	FLUORENE	60	53.3	10		89	50 - 112%
7005-72-3	4-CHLOROPHENYL PHENYL ETHER	60	53	10		88	50 - 111%
100-01-6	4-NITROANILINE	60	55.2	20		92	36 - 118%
103-33-3	AZOBENZENE	60	55.3	10		92	21 - 137%
534-52-1	4,6-DINITRO-2-METHYLPHENOL	60	54.5	20		91	40 - 130%
86-30-6	N-NITROSODIPHENYLAMINE	60	47.4	10		79	48 - 111%
101-55-3	4-BROMOPHENYL PHENYL ETHER	60	52	10		87	52 - 113%
118-74-1	HEXACHLOROBENZENE	60	50.7	10		84	52 - 112%
58-90-2	2,3,4,6-TETRACHLOROPHENOL	100	88.5	10		88	23 - 112%

Data Package ID: SV0903158-1

Date Printed: Tuesday, March 31, 2009

ALS Paragon

LIMS Version: 6.253A

Page 2 of 7

# GC/MS Semi-volatiles

## Method SW8270D

### Laboratory Control Sample and Laboratory Control Sample Duplicate

Lab Name: ALS Paragon

Work Order Number: 0903158

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204503

Lab ID: EX090324-2LCS	Sample Matrix: WATER % Moisture: N/A Date Collected: N/A Date Extracted: 03/24/2009 Date Analyzed: 03/28/2009 Prep Method: SW3520C	Prep Batch: EX090324-2 QCBatchID: EX090324-2-1 Run ID: SV090328-1 Cleanup: NONE Basis: N/A File Name: N5704	Sample Aliquot: 1000 ml Final Volume: 1 ml Result Units: UG/L Clean DF: 1
-----------------------	---	--	--

CASNO	Target Analyte	Spike Added	LCS Result	Reporting Limit	Result Qualifier	LCS % Rec.	Control Limits
87-86-5	PENTACHLOROPHENOL	60	53.1	20		88	38 - 117%
85-01-8	PHENANTHRENE	60	55	10		92	51 - 117%
120-12-7	ANTHRACENE	60	54.4	10		91	54 - 112%
86-74-8	CARBAZOLE	60	56.7	10		95	48 - 117%
84-74-2	DI-N-BUTYL PHTHALATE	60	55.8	10		93	54 - 116%
206-44-0	FLUORANTHENE	60	53.8	10		90	54 - 116%
129-00-0	PYRENE	60	52.6	10		88	49 - 128%
85-68-7	BUTYL BENZYL PHTHALATE	60	54.9	10		92	46 - 116%
56-55-3	BENZO(A)ANTHRACENE	60	54.2	10		90	56 - 109%
91-94-1	3,3'-DICHLOROBENZIDINE	60	28.2	10		47	19 - 111%
218-01-9	CHRYSENE	60	55.6	10		93	55 - 109%
117-81-7	BIS(2-ETHYLHEXYL)PHTHALATE	60	55.4	10		92	42 - 126%
117-84-0	DI-N-OCTYL PHTHALATE	60	55.7	10		93	37 - 137%
205-99-2	BENZO(B)FLUORANTHENE	60	54.9	10		92	45 - 118%
207-08-9	BENZO(K)FLUORANTHENE	60	55.9	10		93	45 - 124%
50-32-8	BENZO(A)PYRENE	60	49.5	10		83	53 - 110%
193-39-5	INDENO(1,2,3-CD)PYRENE	60	56.3	10		94	43 - 125%
53-70-3	DIBENZO(A,H)ANTHRACENE	60	58.6	10		98	42 - 127%
191-24-2	BENZO(G,H,I)PERYLENE	60	57	10		95	38 - 123%

Data Package ID: SV0903158-1

Date Printed: Tuesday, March 31, 2009

ALS Paragon

LIMS Version: 6.253A

Page 3 of 7

# GC/MS Semi-volatiles

## Method SW8270D

### Laboratory Control Sample and Laboratory Control Sample Duplicate

Lab Name: ALS Paragon

Work Order Number: 0903158

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204503

Lab ID: EX090324-2LCSD	Sample Matrix: WATER % Moisture: N/A Date Collected: N/A Date Extracted: 03/24/2009 Date Analyzed: 03/28/2009 Prep Method: SW3520C	Prep Batch: EX090324-2 QCBatchID: EX090324-2-1 Run ID: SV090328-1 Cleanup: NONE Basis: N/A File Name: N5705	Sample Aliquot: 1000 ml Final Volume: 1 ml Result Units: UG/L Clean DF: 1
------------------------	---	--	--

CASNO	Target Analyte	Spike Added	LCSD Result	Reporting Limit	Result Qualifier	LCSD % Rec.	RPD Limit	RPD
110-86-1	PYRIDINE	60	40	10		67	20	5
62-75-9	N-NITROSODIMETHYLAMINE	60	54.1	10		90	20	1
62-53-3	ANILINE	60	45.9	10		76	20	9
108-95-2	PHENOL	60	53	10		88	20	2
111-44-4	BIS(2-CHLOROETHYL)ETHER	60	53.5	10		89	20	3
95-57-8	2-CHLOROPHENOL	60	50.9	10		85	20	2
541-73-1	1,3-DICHLOROBENZENE	60	47.7	10		79	20	4
106-46-7	1,4-DICHLOROBENZENE	60	47.8	10		80	20	4
95-50-1	1,2-DICHLOROBENZENE	60	49	10		82	20	4
100-51-6	BENZYL ALCOHOL	60	52.7	10		88	20	1
108-60-1	BIS(2-CHLOROISOPROPYL)ETHER	60	51.6	10		86	20	3
95-48-7	2-METHYLPHENOL	60	50.9	10		85	20	1
621-64-7	N-NITROSO-DI-N-PROPYLAMINE	60	52.7	10		88	20	1
108-39-4	3+4-METHYLPHENOL	60	50	10		83	20	1
67-72-1	HEXACHLOROETHANE	60	47.3	10		79	20	4
98-95-3	NITROBENZENE	60	34.2	10		57	20	6
78-59-1	ISOPHORONE	60	46.6	10		78	20	2
88-75-5	2-NITROPHENOL	60	46.7	10		78	20	5
105-67-9	2,4-DIMETHYLPHENOL	60	38	10		63	20	10
111-91-1	BIS(2-CHLOROETHOXY)METHANE	60	47.4	10		79	20	3
120-83-2	2,4-DICHLOROPHENOL	60	46.8	10		78	20	4
65-85-0	BENZOIC ACID	100	34.7	50	J	35	20	19
120-82-1	1,2,4-TRICHLOROBENZENE	60	41.9	10		70	20	6
91-20-3	NAPHTHALENE	60	45.4	10		76	20	4
106-47-8	4-CHLOROANILINE	60	44.9	10		75	20	1
87-68-3	HEXACHLOROBUTADIENE	60	40	10		67	20	6
59-50-7	4-CHLORO-3-METHYLPHENOL	60	49.2	10		82	20	1

Data Package ID: SV0903158-1

Date Printed: Tuesday, March 31, 2009

ALS Paragon

LIMS Version: 6.253A

Page 4 of 7

# GC/MS Semi-volatiles

## Method SW8270D

### Laboratory Control Sample and Laboratory Control Sample Duplicate

Lab Name: ALS Paragon

Work Order Number: 0903158

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204503

Lab ID: EX090324-2LCSD	Sample Matrix: WATER % Moisture: N/A Date Collected: N/A Date Extracted: 03/24/2009 Date Analyzed: 03/28/2009 Prep Method: SW3520C	Prep Batch: EX090324-2 QCBatchID: EX090324-2-1 Run ID: SV090328-1 Cleanup: NONE Basis: N/A File Name: N5705	Sample Aliquot: 1000 ml Final Volume: 1 ml Result Units: UG/L Clean DF: 1
------------------------	---	--	--

CASNO	Target Analyte	Spike Added	LCSD Result	Reporting Limit	Result Qualifier	LCSD % Rec.	RPD Limit	RPD
91-57-6	2-METHYLNAPHTHALENE	60	44.6	10		74	20	3
90-12-0	1-METHYLNAPHTHALENE	60	50.7	10		85	20	2
77-47-4	HEXACHLOROCYCLOPENTADIENE	60	15.3	10		26	20	10
88-06-2	2,4,6-TRICHLOROPHENOL	60	52.4	10		87	20	1
95-95-4	2,4,5-TRICHLOROPHENOL	60	54	10		90	20	1
91-58-7	2-CHLORONAPHTHALENE	60	51	10		85	20	1
88-74-4	2-NITROANILINE	60	58.9	20		98	20	1
131-11-3	DIMETHYL PHTHALATE	60	53.1	10		89	20	1
606-20-2	2,6-DINITROTOLUENE	60	55.7	10		93	20	1
208-96-8	ACENAPHTHYLENE	60	53.8	10		90	20	0
99-09-2	3-NITROANILINE	60	56.7	20		95	20	3
83-32-9	ACENAPHTHENE	60	52.8	10		88	20	0
51-28-5	2,4-DINITROPHENOL	60	51.6	20		86	20	0
100-02-7	4-NITROPHENOL	60	48.9	20		81	20	6
132-64-9	DIBENZOFURAN	60	52.7	10		88	20	1
121-14-2	2,4-DINITROTOLUENE	60	52.4	10		87	20	4
84-66-2	DIETHYL PHTHALATE	60	54.3	10		91	20	4
86-73-7	FLUORENE	60	52.2	10		87	20	2
7005-72-3	4-CHLOROPHENYL PHENYL ETHER	60	52.3	10		87	20	1
100-01-6	4-NITROANILINE	60	51.3	20		86	20	7
103-33-3	AZOBENZENE	60	53.2	10		89	20	4
534-52-1	4,6-DINITRO-2-METHYLPHENOL	60	54.9	20		92	20	1
86-30-6	N-NITROSODIPHENYLAMINE	60	46.5	10		77	20	2
101-55-3	4-BROMOPHENYL PHENYL ETHER	60	53.1	10		89	20	2
118-74-1	HEXACHLOROBENZENE	60	52.1	10		87	20	3
58-90-2	2,3,4,6-TETRACHLOROPHENOL	100	89.6	10		90	20	1
87-86-5	PENTACHLOROPHENOL	60	53	20		88	20	0

Data Package ID: SV0903158-1

Date Printed: Tuesday, March 31, 2009

ALS Paragon

LIMS Version: 6.253A

Page 5 of 7

# GC/MS Semi-volatiles

## Method SW8270D

### Laboratory Control Sample and Laboratory Control Sample Duplicate

Lab Name: ALS Paragon

Work Order Number: 0903158

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204503

Lab ID: EX090324-2LCSD	Sample Matrix: WATER % Moisture: N/A Date Collected: N/A Date Extracted: 03/24/2009 Date Analyzed: 03/28/2009 Prep Method: SW3520C	Prep Batch: EX090324-2 QCBatchID: EX090324-2-1 Run ID: SV090328-1 Cleanup: NONE Basis: N/A File Name: N5705	Sample Aliquot: 1000 ml Final Volume: 1 ml Result Units: UG/L Clean DF: 1
------------------------	---	--	--

CASNO	Target Analyte	Spike Added	LCSD Result	Reporting Limit	Result Qualifier	LCSD % Rec.	RPD Limit	RPD
85-01-8	PHENANTHRENE	60	54.6	10		91	20	1
120-12-7	ANTHRACENE	60	54.2	10		90	20	0
86-74-8	CARBAZOLE	60	54.9	10		92	20	3
84-74-2	DI-N-BUTYL PHTHALATE	60	54.9	10		91	20	2
206-44-0	FLUORANTHENE	60	53.4	10		89	20	1
129-00-0	PYRENE	60	52.5	10		87	20	0
85-68-7	BUTYL BENZYL PHTHALATE	60	55.5	10		92	20	1
56-55-3	BENZO(A)ANTHRACENE	60	54.5	10		91	20	1
91-94-1	3,3'-DICHLOROBENZIDINE	60	26.5	10		44	20	6
218-01-9	CHRYSENE	60	54.6	10		91	20	2
117-81-7	BIS(2-ETHYLHEXYL)PHTHALATE	60	55.7	10		93	20	1
117-84-0	DI-N-OCTYL PHTHALATE	60	55.5	10		92	20	1
205-99-2	BENZO(B)FLUORANTHENE	60	57.2	10		95	20	4
207-08-9	BENZO(K)FLUORANTHENE	60	56.2	10		94	20	0
50-32-8	BENZO(A)PYRENE	60	49.3	10		82	20	0
193-39-5	INDENO(1,2,3-CD)PYRENE	60	54.3	10		91	20	4
53-70-3	DIBENZO(A,H)ANTHRACENE	60	56.2	10		94	20	4
191-24-2	BENZO(G,H,I)PERYLENE	60	53.6	10		89	20	6

Data Package ID: SV0903158-1

Date Printed: Tuesday, March 31, 2009

ALS Paragon

LIMS Version: 6.253A

Page 6 of 7

# GC/MS Semi-volatiles

Method SW8270D

## Laboratory Control Sample and Laboratory Control Sample Duplicate

Lab Name: ALS Paragon

Work Order Number: 0903158

Client Name: Colorado Oil & Gas Conservation Commission

ClientProject ID: Complaint 200204503

---

### Surrogate Recovery LCS/LCSD

CASNO	Target Analyte	Spike Added	LCS % Rec.	LCS Flag	LCSD % Rec.	LCSD Flag	Control Limits
118-79-6	2,4,6-TRIBROMOPHENOL	75	85		84		23 - 100
321-60-8	2-FLUOROBIPHENYL	50	83		84		21 - 106
367-12-4	2-FLUOROPHENOL	75	82		86		21 - 100
4165-60-0	NITROBENZENE-D5	50	74		79		34 - 111
4165-62-2	PHENOL-D5	75	86		88		15 - 104
1718-51-0	TERPHENYL-D14	50	85		85		33 - 111

---

Data Package ID: SV0903158-1

---

Date Printed: Tuesday, March 31, 2009

ALS Paragon

LIMS Version: 6.253A

Page 7 of 7

## Quantitation Report (Not Reviewed)

Data File : D:\HPCHEM\1\DATA\032809\N5703.D  
 Acq On : 28 Mar 2009 3:25 pm  
 Sample : EX090324-2MB  
 Misc : WATER EX090324-2  
 MS Integration Params: RTEINT.P  
 Quant Time: Mar 28 15:51 2009

Vial: 3  
 Operator: JK SOP 506 Rev  
 Inst : GC/MS Ins  
 Multiplr: 1.00

Quant Results File: 032709S1.RES

Quant Method : D:\HPCHEM\1\METHODS\032709S1.M (RTE Integrator)

Title : GC-MS Semivolatiles SOP no. 506

Last Update : Sat Mar 28 14:34:56 2009

Response via : Initial Calibration

DataAcq Meth : 032709S1

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	5.94	152	287635	40.00	ng/uL	0.00
24) Naphthalene-d8	7.14	136	1031485	40.00	ng/uL	0.00
41) Acenaphthene-d10	8.69	164	490555	40.00	ng/uL	0.00
69) Phenanthrene-d10	9.98	188	748538	40.00	ng/uL	0.00
80) Chrysene-d12	12.27	240	813035	40.00	ng/uL	0.00
91) Perylene-d12	13.84	264	609639	40.00	ng/uL	0.00

## System Monitoring Compounds

5) 2-Fluorophenol	4.54	112	574460	70.71	ng/uL	0.00
Spiked Amount 75.000	Range 21 - 100		Recovery	=	94.28%	
6) 2-Chlorophenol-d4	5.71	132	583164	69.33	ng/uL	0.00
Spiked Amount 75.000	Range 33 - 110		Recovery	=	92.44%	
8) Phenol-d5	5.51	99	722788	71.64	ng/uL	-0.01
Spiked Amount 75.000	Range 15 - 104		Recovery	=	95.52%	
15) 1,2-Dichlorobenzene-d4	6.09	152	279635	44.87	ng/uL	0.00
Spiked Amount 50.000	Range 16 - 110		Recovery	=	89.74%	
25) Nitrobenzene-d5	6.46	82	417511	46.96	ng/uL	0.00
Spiked Amount 50.000	Range 34 - 111		Recovery	=	93.92%	
46) 2-Fluorobiphenyl	8.07	172	777809	45.36	ng/uL	0.00
Spiked Amount 50.000	Range 21 - 106		Recovery	=	90.72%	
68) 2,4,6-Tribromophenol	9.37	330	96111	49.94	ng/uL	0.00
Spiked Amount 75.000	Range 23 - 100		Recovery	=	66.59%	
83) p-Terphenyl-d14	11.30	244	784660	51.04	ng/uL	0.00
Spiked Amount 50.000	Range 33 - 111		Recovery	=	102.08%	

## Target Compounds

Qvalue

(#) = qualifier out of range (m) = manual integration  
 N5703.D 032709S1.M Sat Mar 28 15:51:34 2009

JL  
3-21-09

Page 1


# Quantitation Report

Data File : D:\HPCHEM\1\DATA\032809\N5703.D  
 Acq On : 28 Mar 2009 3:25 pm  
 Sample : EX090324-2MB  
 Misc : WATER EX090324-2  
 MS Integration Params: RTEINT.P  
 Quant Time: Mar 28 15:51 2009

Vial: 3  
 Operator: JK SOP 506  
 Inst : GC/MS Ins  
 Multiplr: 1.00

Quant Results File: 032709S1.RES

Method : D:\HPCHEM\1\METHODS\032709S1.M (RTE Integrator)  
 Title : GC-MS Semivolatiles SOP no. 506  
 Last Update : Sat Mar 28 14:34:56 2009  
 Response via : Initial Calibration



# Library Search Compound Report

Data File : D:\HPCHEM\1\DATA\032809\N5703.D  
 Acq On : 28 Mar 2009 3:25 pm  
 Sample : EX090324-2MB  
 Misc : WATER EX090324-2  
 MS Integration Params: LSCINT.P


Vial: 3  
 Operator: JK SOP 50  
 Inst : GC/MS Ins  
 Multipllr: 1.00

Quant Method : D:\HPCHEM\1\METHODS\032709S1.M (RTE Integrator)  
 Title : GC-MS Semivolatiles SOP no. 506  
 Library : D:\DATABASE\NIST98.L

\*\*\*\*\*

Peak Number 1 Amylene Hydrate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.		
3.91	10.75 ng/uL	471644	1,4-Dichlorobenzene-d4	5.94		
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Amylene Hydrate		88	C5H12O	000075-85-4	40
2	3-Hydroxy-3-methyl-2-butanone		102	C5H10O2	000115-22-0	38
3	4-Pentene-2-ol, 2-methyl		100	C6H12O	000624-97-5	36
4	Formamide, N-methyl-		59	C2H5NO	000123-39-7	9

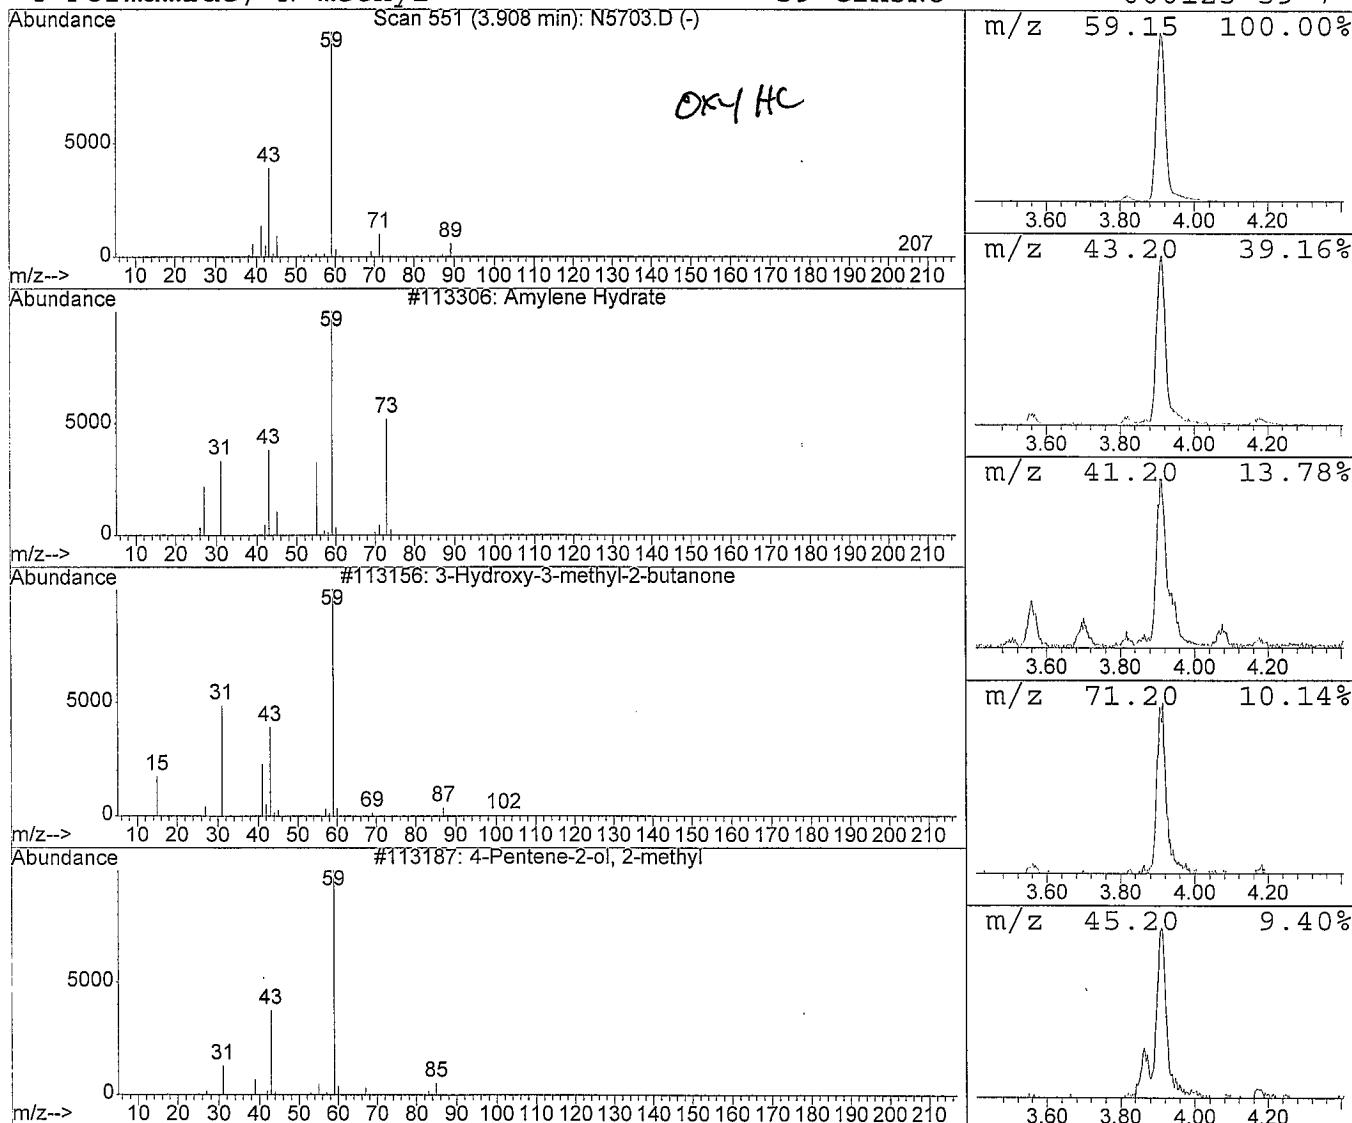

Data File : D:\HPCHEM\1\DATA\032809\N5708.D  
 Acq On : 28 Mar 2009 5:25 pm  
 Sample : 0903158-1  
 Misc : WATER EX090324-2  
 MS Integration Params: RTEINT.P  
 Quant Time: Mar 30 8:51 2009

Vial: 8  
 Operator: JK SOP 506 Rev  
 Inst : GC/MS Ins  
 Multiplr: 1.00

Quant Results File: 032709S1.RES

Quant Method : D:\HPCHEM\1\METHODS\032709S1.M (RTE Integrator)

Title : GC-MS Semivolatiles SOP no. 506

Last Update : Sat Mar 28 14:34:56 2009

Response via : Initial Calibration

DataAcq Meth : 032709S1

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	5.94	152	335512✓	40.00	ng/uL	0.00
24) Naphthalene-d8	7.14	136	1214961✓	40.00	ng/uL	0.00
41) Acenaphthene-d10	8.69	164	564314✓	40.00	ng/uL	-0.01
69) Phenanthrene-d10	9.97	188	892707✓	40.00	ng/uL	-0.01
80) Chrysene-d12	12.27	240	1044829✓	40.00	ng/uL	-0.01
91) Perylene-d12	13.84	264	770035✓	40.00	ng/uL	0.00

## System Monitoring Compounds

5) 2-Fluorophenol	4.54	112	594540	62.74	ng/uL	0.00
Spiked Amount 75.000	Range 21 - 100		Recovery	=	83.65%	✓
6) 2-Chlorophenol-d4	5.71	132	615735	62.76	ng/uL	-0.01
Spiked Amount 75.000	Range 33 - 110		Recovery	=	83.68%	
8) Phenol-d5	5.51	99	765916	65.08	ng/uL	-0.01
Spiked Amount 75.000	Range 15 - 104		Recovery	=	86.77%	✓
15) 1,2-Dichlorobenzene-d4	6.09	152	295708	40.68	ng/uL	0.00
Spiked Amount 50.000	Range 16 - 110		Recovery	=	81.36%	
25) Nitrobenzene-d5	6.46	82	448514	42.83	ng/uL	-0.01
Spiked Amount 50.000	Range 34 - 111		Recovery	=	85.66%	✓
46) 2-Fluorobiphenyl	8.07	172	856426	43.42	ng/uL	0.00
Spiked Amount 50.000	Range 21 - 106		Recovery	=	86.84%	✓
68) 2,4,6-Tribromophenol	9.37	330	108645	49.22	ng/uL	0.00
Spiked Amount 75.000	Range 23 - 100		Recovery	=	65.63%	✓
83) p-Terphenyl-d14	11.30	244	929017	47.02	ng/uL	0.00
Spiked Amount 50.000	Range 33 - 111		Recovery	=	94.04%	✓

## Target Compounds

Qvalue

(#) = qualifier out of range (m) = manual integration  
 N5708.D 032709S1.M Mon Mar 30 08:51:44 2009

91  
3-1-09

Page 1


Quantitation Report

Data File : D:\HPCHEM\1\DATA\032809\N5708.D  
 Acq On : 28 Mar 2009 5:25 pm  
 Sample : 0903158-1  
 Misc : WATER EX090324-2  
 MS Integration Params: RTEINT.P  
 Quant Time: Mar 30 8:51 2009

Vial: 8  
 Operator: JK SOP 506  
 Inst : GC/MS Ins  
 Multiplr: 1.00

Quant Results File: 032709S1.RES

Method : D:\HPCHEM\1\METHODS\032709S1.M (RTE Integrator)  
 Title : GC-MS Semivolatiles SOP no. 506  
 Last Update : Sat Mar 28 14:34:56 2009  
 Response via : Initial Calibration



## Library Search Compound Report

Data File : D:\HPCHEM\1\DATA\032809\N5708.D  
 Acq On : 28 Mar 2009 5:25 pm  
 Sample : 0903158-1  
 Misc : WATER EX090324-2  
 MS Integration Params: LSCINT.P

Vial: 8  
 Operator: JK SOP 50  
 Inst : GC/MS Ins  
 Multiplr: 1.00

Quant Method : D:\HPCHEM\1\METHODS\032709S1.M (RTE Integrator)  
 Title : GC-MS Semivolatiles SOP no. 506  
 Library : D:\DATABASE\NIST98.L

\*\*\*\*\*  
 Peak Number 1 3-Hydroxy-3-methyl-2-butanone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.		
3.91	19.63 ng/uL	987075	1,4-Dichlorobenzene-d4	5.94		
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Hydroxy-3-methyl-2-butanone	102	C5H10O2	000115-22-0	45	
2	Amylene Hydrate	88	C5H12O	000075-85-4	39	
3	1,2-Butanediol	90	C4H10O2	000584-03-2	38	
4	2-Propanol, 1-methoxy-2-methyl-	104	C5H12O2	003587-64-2	9	

