
MAIN PASS
MAIN PASS
MAIN PASS

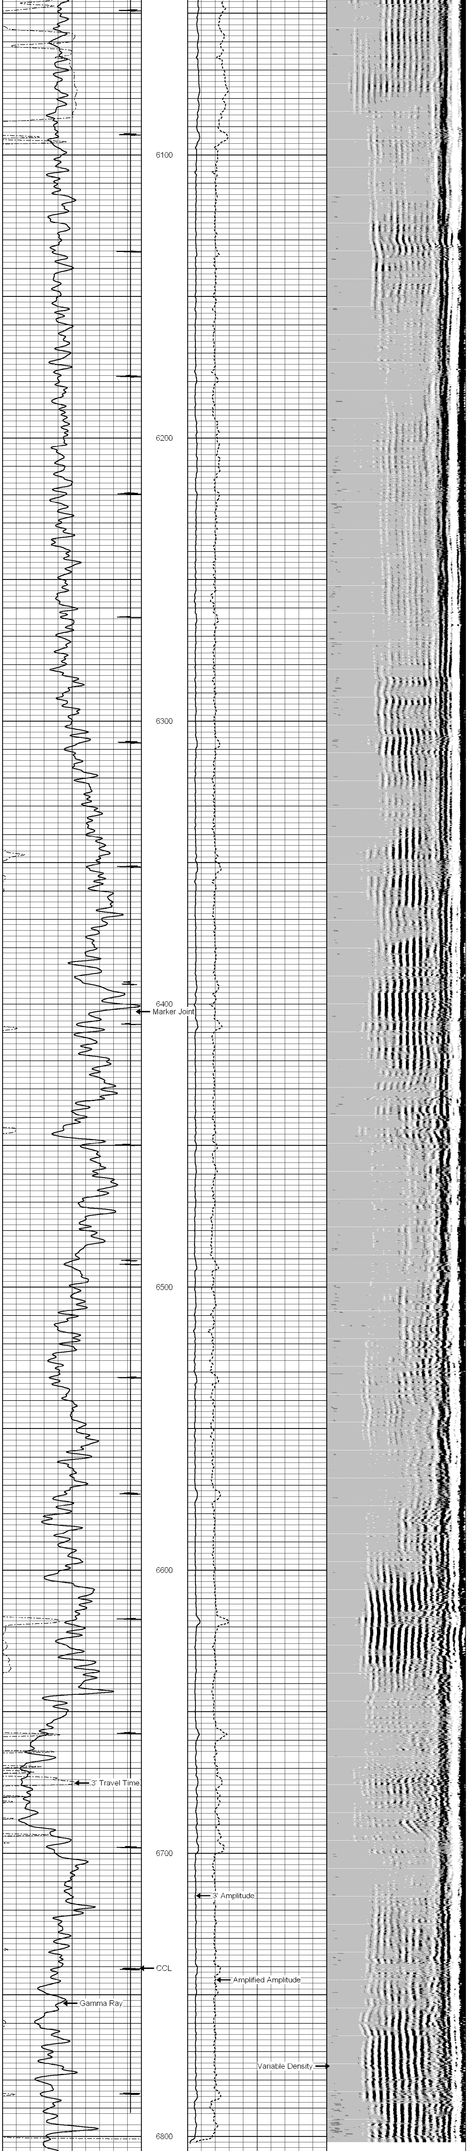

Calibration Report

Database File: antelope 32-19.db
Dataset Pathname: pass5
Dataset Creation: Tue Mar 29 08:43:53 2011 by Log Std Casedhole 10121

Gamma Ray Calibration Report

Serial Number:	576	
Tool Model:	1.69TEKCO	
Performed:	Sun Jun 13 13:33:21 1993	
Calibrator Value:	1.0	GAPI
Background Reading:	0.0	cps
Calibrator Reading:	1.0	cps
Sensitivity:	1.0000	GAPI/cps

Cement Bond Log Calibration Report

Serial Number:	1		
Tool Model:	3-Stelco169		
Performed:	Tue Mar 29 07:44:57 2011		
Depth:	3093.72	ft	
Casing Diameter:	4.5	in	
	3' Spacing	5' Spacing	
Signal Zero:	3	6	mV
Calibrated Amplitude:	81.1961	81.1961	mV
Reading at Signal Zero:	0.03	0.03	V
Reading in Free Pipe:	2.05413	2.5	V
Gain:	38.632	32.8729	
Offset:	1.84104	-0.986187	