
MAIN PASS
MAIN PASS
MAIN PASS
MAIN PASS

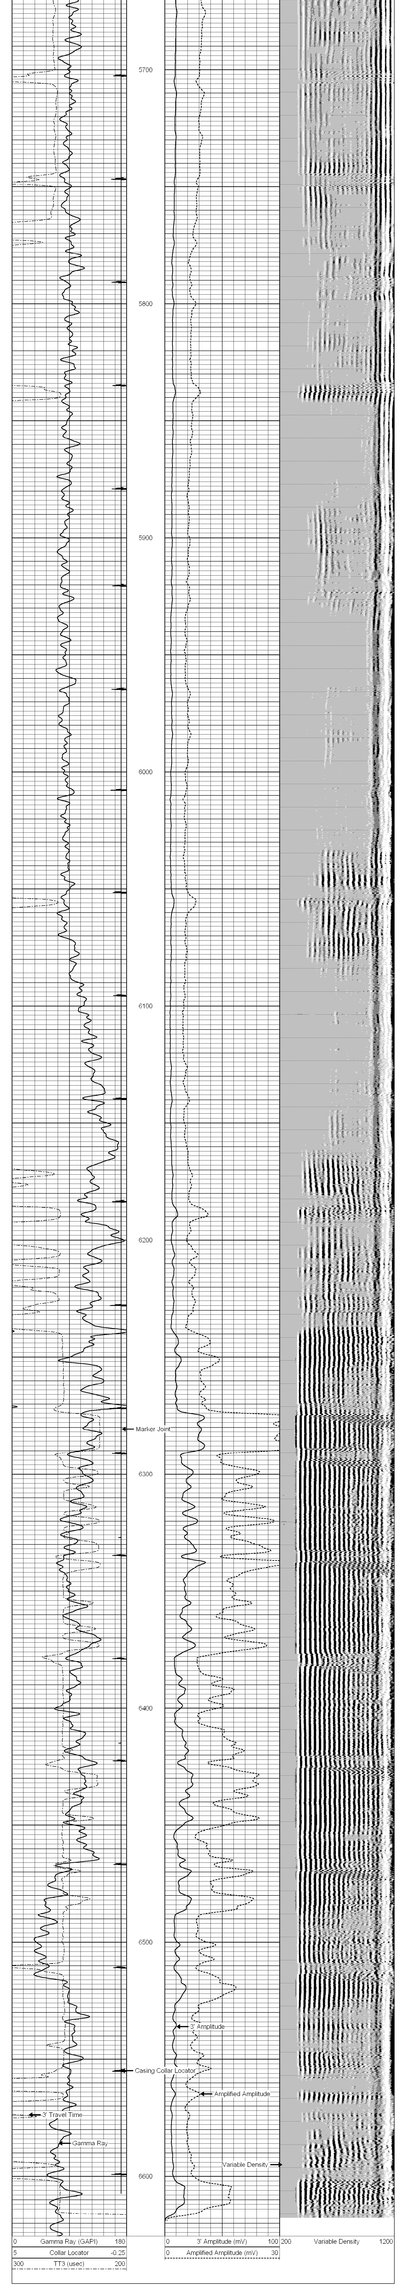

0	Gamma Ray (GAPI)	180	0	3' Amplitude (mV) 100,200	Variable Density 1200
-5	Collar Locator	0.25	0	Amplified Amplitude (mV) 30	
300	TT3 (usec)	200			

Calibration Report

Database File:	antelope 41-31_cbl.db
Dataset Pathname:	pass1
Dataset Creation:	Tue Jul 12 09:39:37 2011 by Log Std Casedhole 10121

Gamma Ray Calibration Report

Serial Number:	576	
Tool Model:	1.69TEKCO	
Performed:	Sun Jun 13 13:33:21 1993	
Calibrator Value:	1.0	GAPI
Background Reading:	0.0	cps
Calibrator Reading:	1.0	cps
Sensitivity:	1.0000	GAPI/cps

Cement Bond Log Calibration Report

Serial Number:	1		
Tool Model:	3-Stekco169		
Performed:	Tue Jul 12 09:23:12 2011		
Depth:	2494.15	ft	
Casing Diameter:	4.5	in	
	3' Spacing	5' Spacing	
Signal Zero:	3	0	mV
Calibrated Amplitude:	81.1961	81.1961	mV
Reading at Signal Zero:	0.06	0.03	V
Reading in Free Pipe:	2.01465	2.41577	V
Gain:	40.0052	34.0335	
Offset:	0.599688	-1.021	