
Nihon Kohden
QUANN-ROU CO.,
SLEEP SCAN 32L
Name
Date
Time
Comment
Total
Sleep
Awake
Stage 1
Stage 2
Stage 3
Stage 4
REM
Movement
Unknown
Sleep Efficiency
Sleep Latency
REM Latency
Awake (%)
Stage 1 (%)
Stage 2 (%)
Stage 3 (%)
Stage 4 (%)
REM (%)
Movement (%)
Unknown (%)
Arousal Index
Apnea Index
Hypopnea Index
AHI
RDI
Desaturation Index
Snore Index
Snore (%)
Position
Supine
Prone
Left
Right
Upright
Unknown
Supine (%)
Prone (%)
Left (%)
Right (%)
Upright (%)
Unknown (%)
Body Position Change
Leg Movement Index
Periodic Leg Movement Index
Periodic Leg Movement Arousal Index
Respiratory Arousal Index
Respiratory Effort Related Arousal Index
Respiratory Effort Related Arousal Index
Cheyne-Stokes Respiration Index
Cheyne-Stokes Respiration (%)
Mean SpO2
Lowest SpO2
Mean Pulse Rate
Lowest Pulse Rate
Highest Pulse Rate
Mean Body Temperature
Lowest Body Temperature
Highest Body Temperature
Mean Room Temperature
Lowest Room Temperature
Highest Room Temperature
Mean Room Humidity
Lowest Room Humidity
Highest Room Humidity
Mean Light Intensity
Lowest Light Intensity
Highest Light Intensity
Mean Noise Level
Lowest Noise Level
Highest Noise Level
Mean Tidal Volume
Lowest Tidal Volume
Highest Tidal Volume
Mean Minute Ventilation
Lowest Minute Ventilation
Highest Minute Ventilation
Mean Respiratory Rate
Lowest Respiratory Rate
Highest Respiratory Rate
Mean Peak Flow
Lowest Peak Flow
Highest Peak Flow
Mean Inspiratory Flow
Lowest Inspiratory Flow
Highest Inspiratory Flow
Mean Expiratory Flow
Lowest Expiratory Flow
Highest Expiratory Flow
Mean Inspiratory Time
Lowest Inspiratory Time
Highest Inspiratory Time
Mean Expiratory Time
Lowest Expiratory Time
Highest Expiratory Time
Mean I:E Ratio
Lowest I:E Ratio
Highest I:E Ratio
Mean Tidal Volume/Kg
Lowest Tidal Volume/Kg
Highest Tidal Volume/Kg
Mean Minute Ventilation/Kg
Lowest Minute Ventilation/Kg
Highest Minute Ventilation/Kg
Mean Peak Flow/Kg
Lowest Peak Flow/Kg
Highest Peak Flow/Kg
Mean Inspiratory Flow/Kg
Lowest Inspiratory Flow/Kg
Highest Inspiratory Flow/Kg
Mean Expiratory Flow/Kg
Lowest Expiratory Flow/Kg
Highest Expiratory Flow/Kg
Mean Inspiratory Time/Kg
Lowest Inspiratory Time/Kg
Highest Inspiratory Time/Kg
Mean Expiratory Time/Kg
Lowest Expiratory Time/Kg
Highest Expiratory Time/Kg
Mean I:E Ratio/Kg
Lowest I:E Ratio/Kg
Highest I:E Ratio/Kg

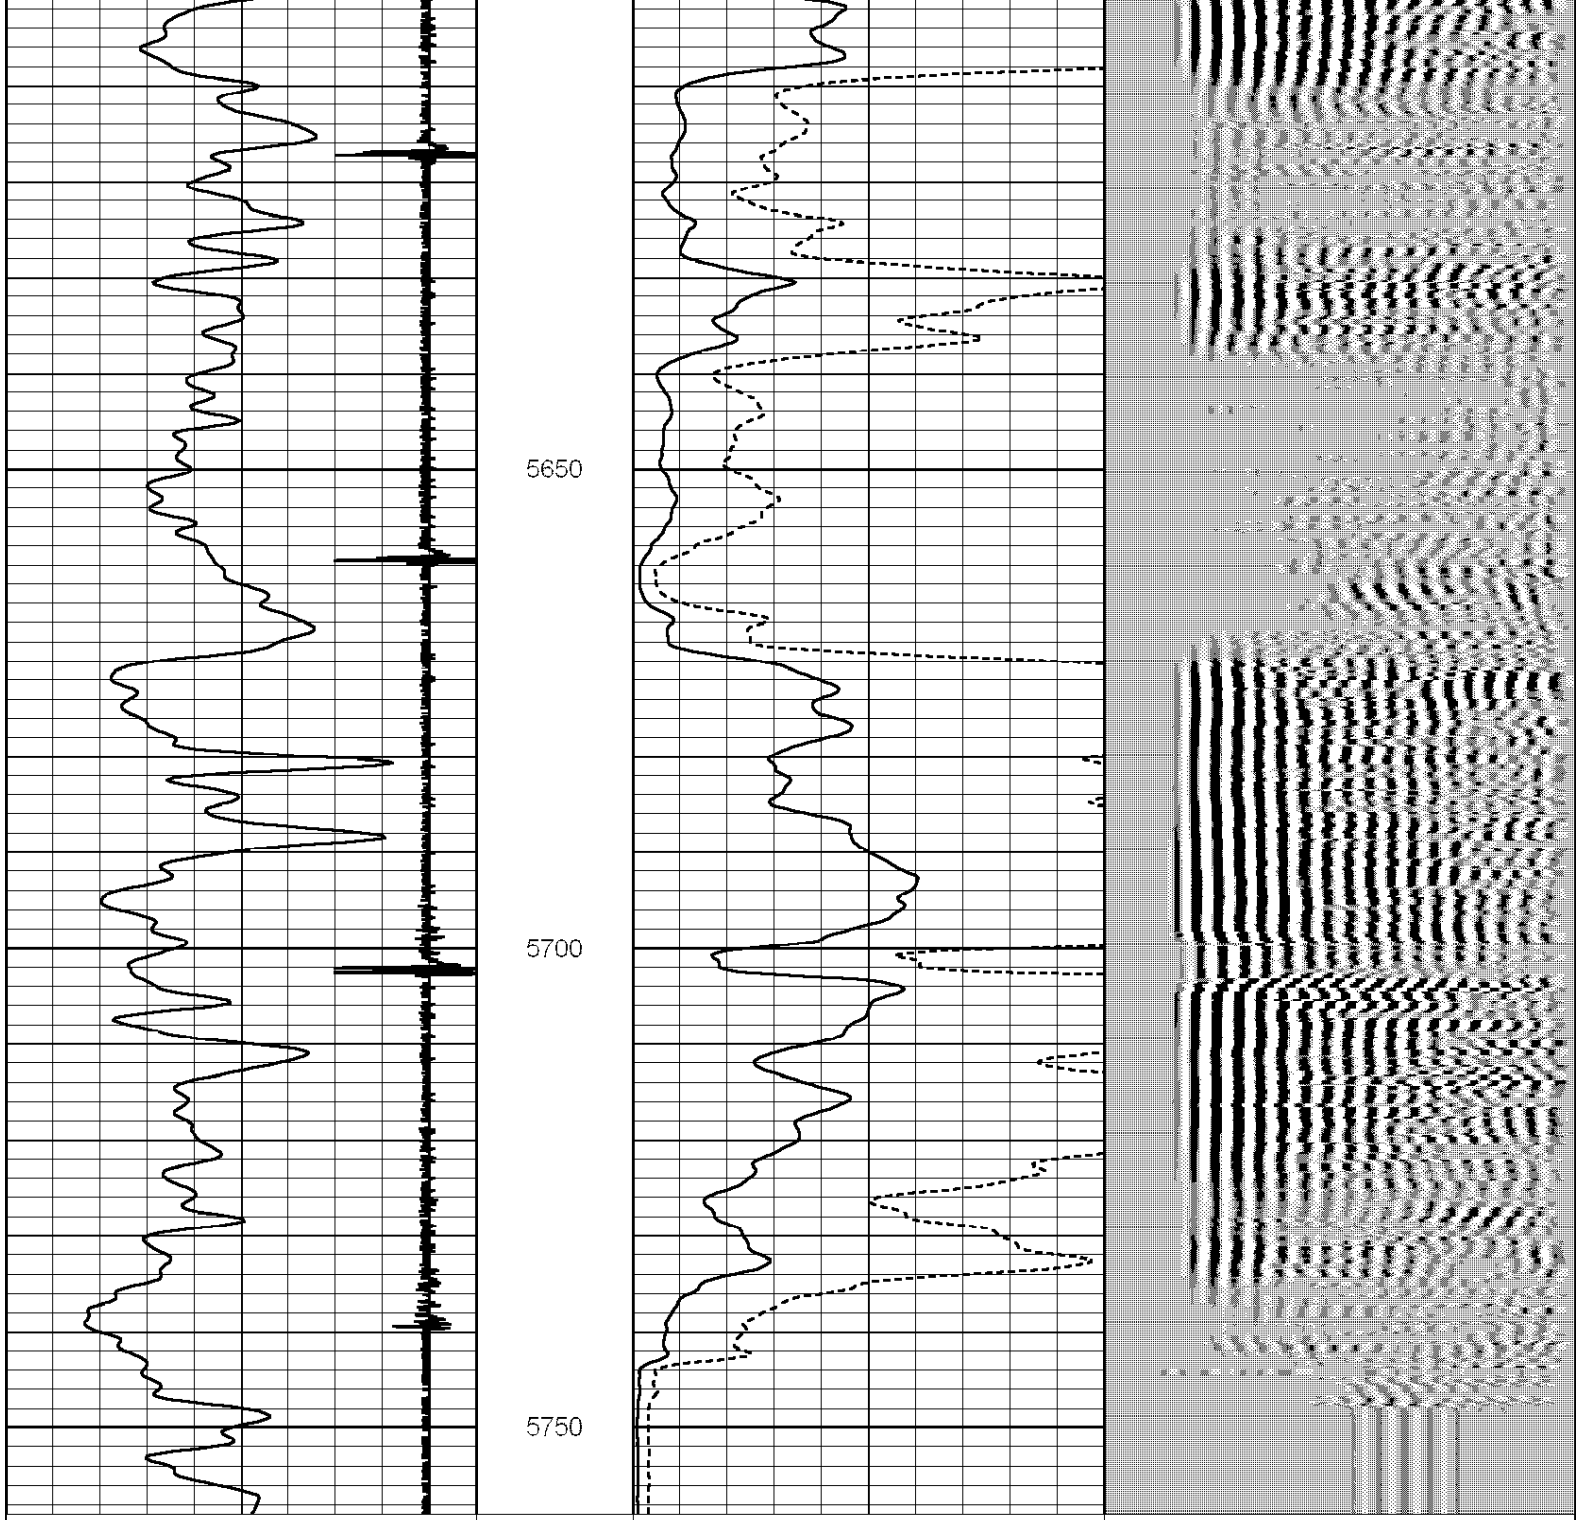
5650
5700
5750
9
Collar Locator
-1
0
Gamma Ray (GAPI)
240
0
Amplitude (mV)
100
200
VDL
1200