


Summit testing services Anadarko MIT Moser 11-28

Gauge Information	
Serial Number	562139
Model	10KPSIXP2I
Message Store	-----
Units	PSI

Run Info	
Start Time	4/13/17 9:27:37 AM
Stop Time	4/13/17 9:47:48 AM
Logging Interval	60

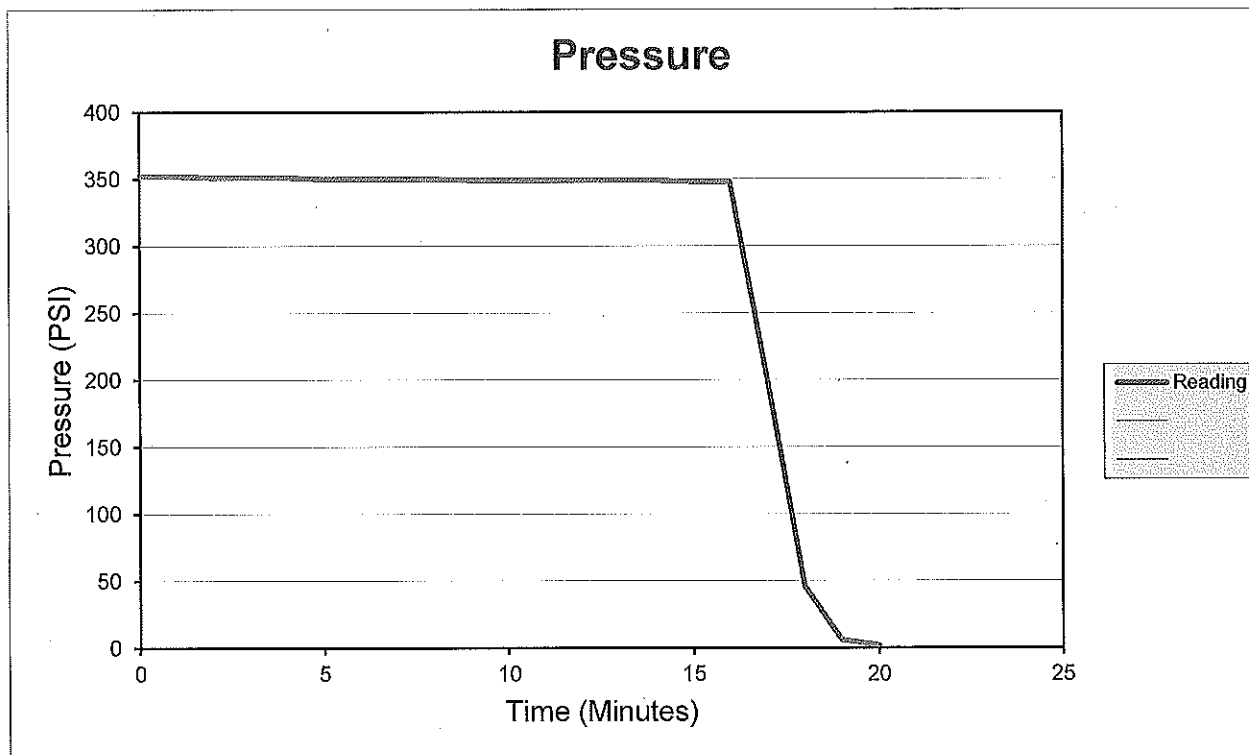

Start Time 4/13/2017 9:27

Stop Time 4/13/2017 9:47

Time	Reading	Time (hour	Time (minutes)
0		0.00	0.00
0		0.00	0.00
0		0.00	0.00
0	352 Start test	0.00	0.00
60	352	0.02	1.00
120	351	0.03	2.00
180	351	0.05	3.00
240	351	0.07	4.00
300	350	0.08	5.00
360	350	0.10	6.00
420	350	0.12	7.00
480	350	0.13	8.00
540	349	0.15	9.00
600	349	0.17	10.00
660	349	0.18	11.00
720	349	0.20	12.00
780	349	0.22	13.00
840	349 End test	0.23	14.00
900	348	0.25	15.00
960	348	0.27	16.00
1020	201	0.28	17.00
1080	46	0.30	18.00
1140	6	0.32	19.00
1200	2	0.33	20.00